

FIG. 1

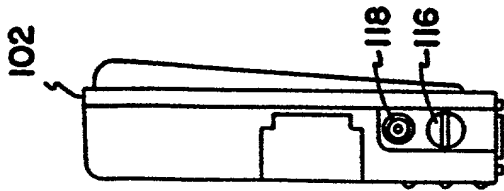


FIG. 1A

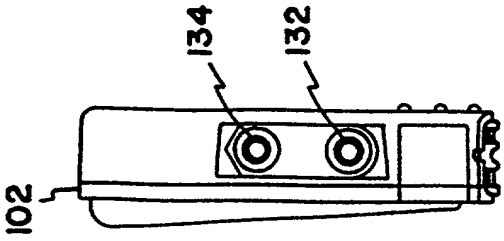


FIG. 1B

FIG. 3

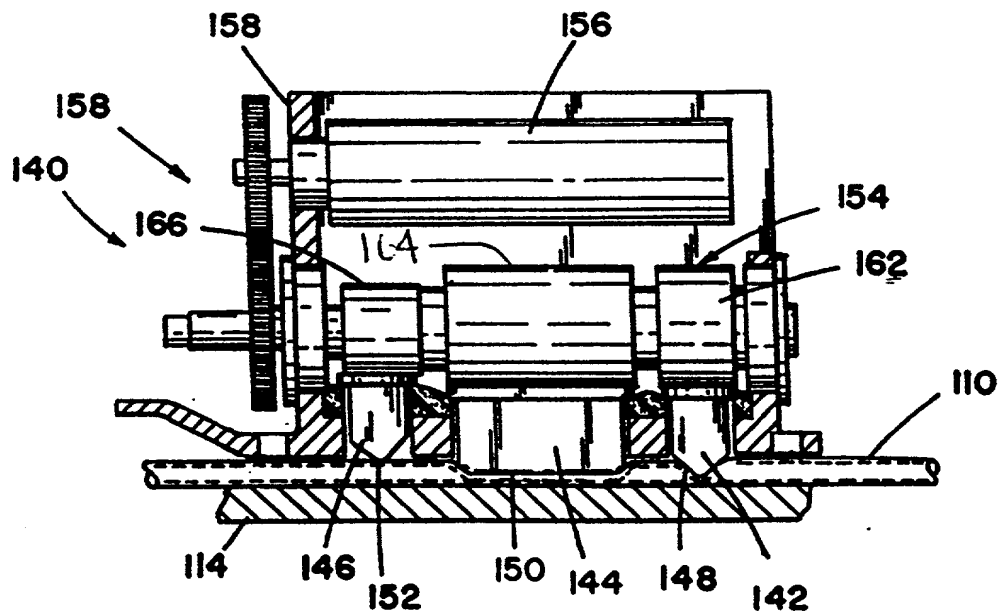
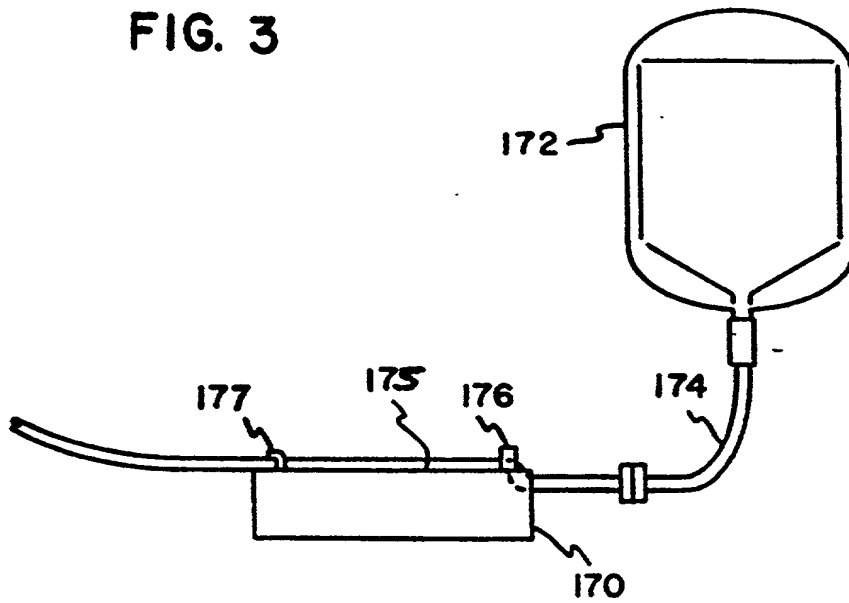


FIG. 2

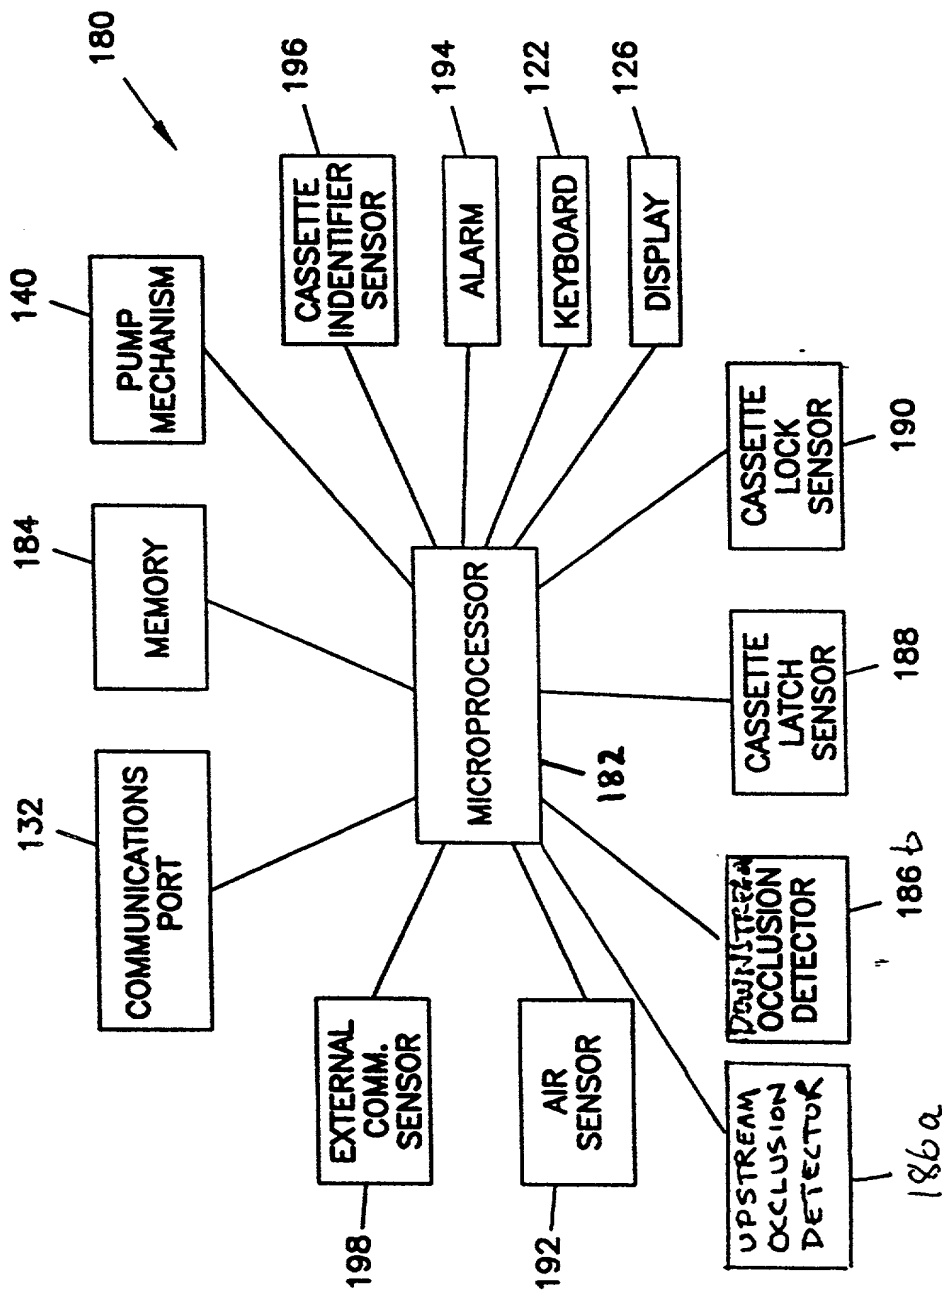


FIG. 4

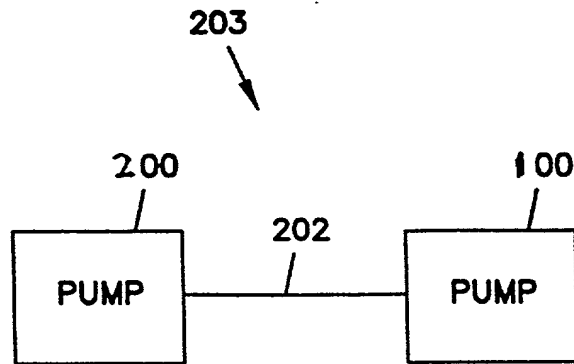


FIG. 5

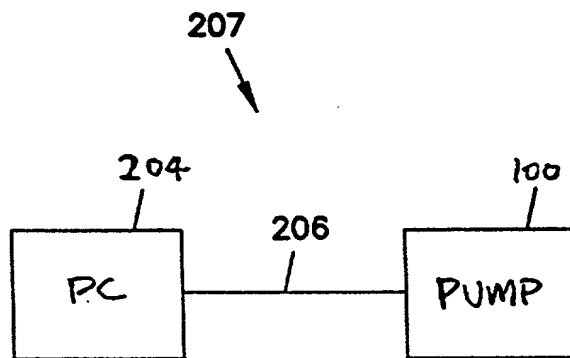


FIG. 6

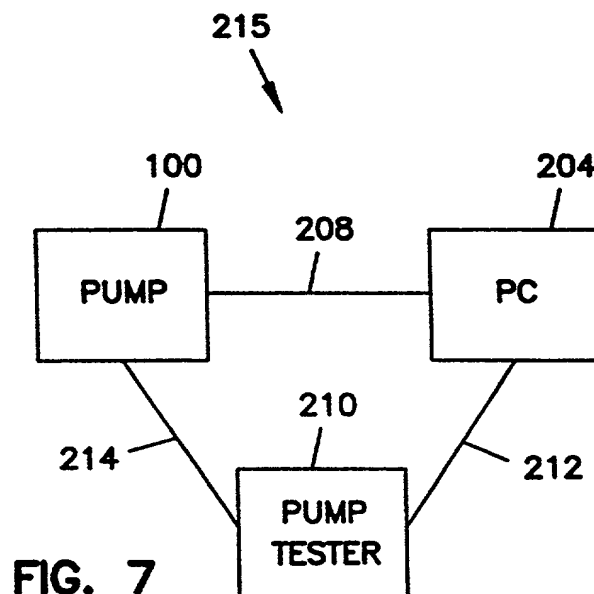


FIG. 7

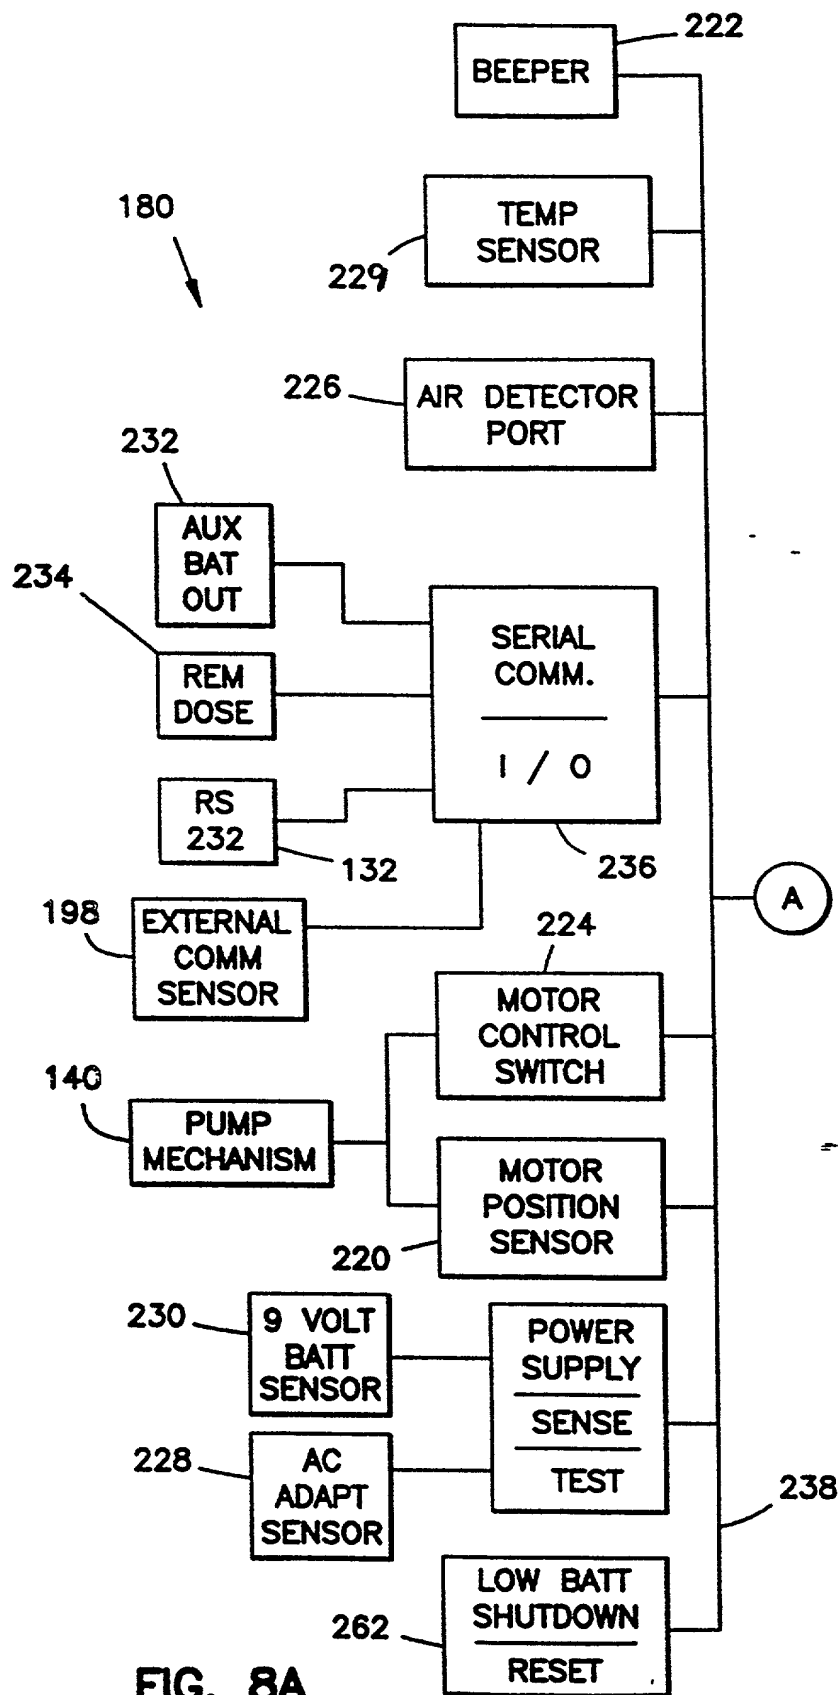


FIG. 8A

10058291 00000000

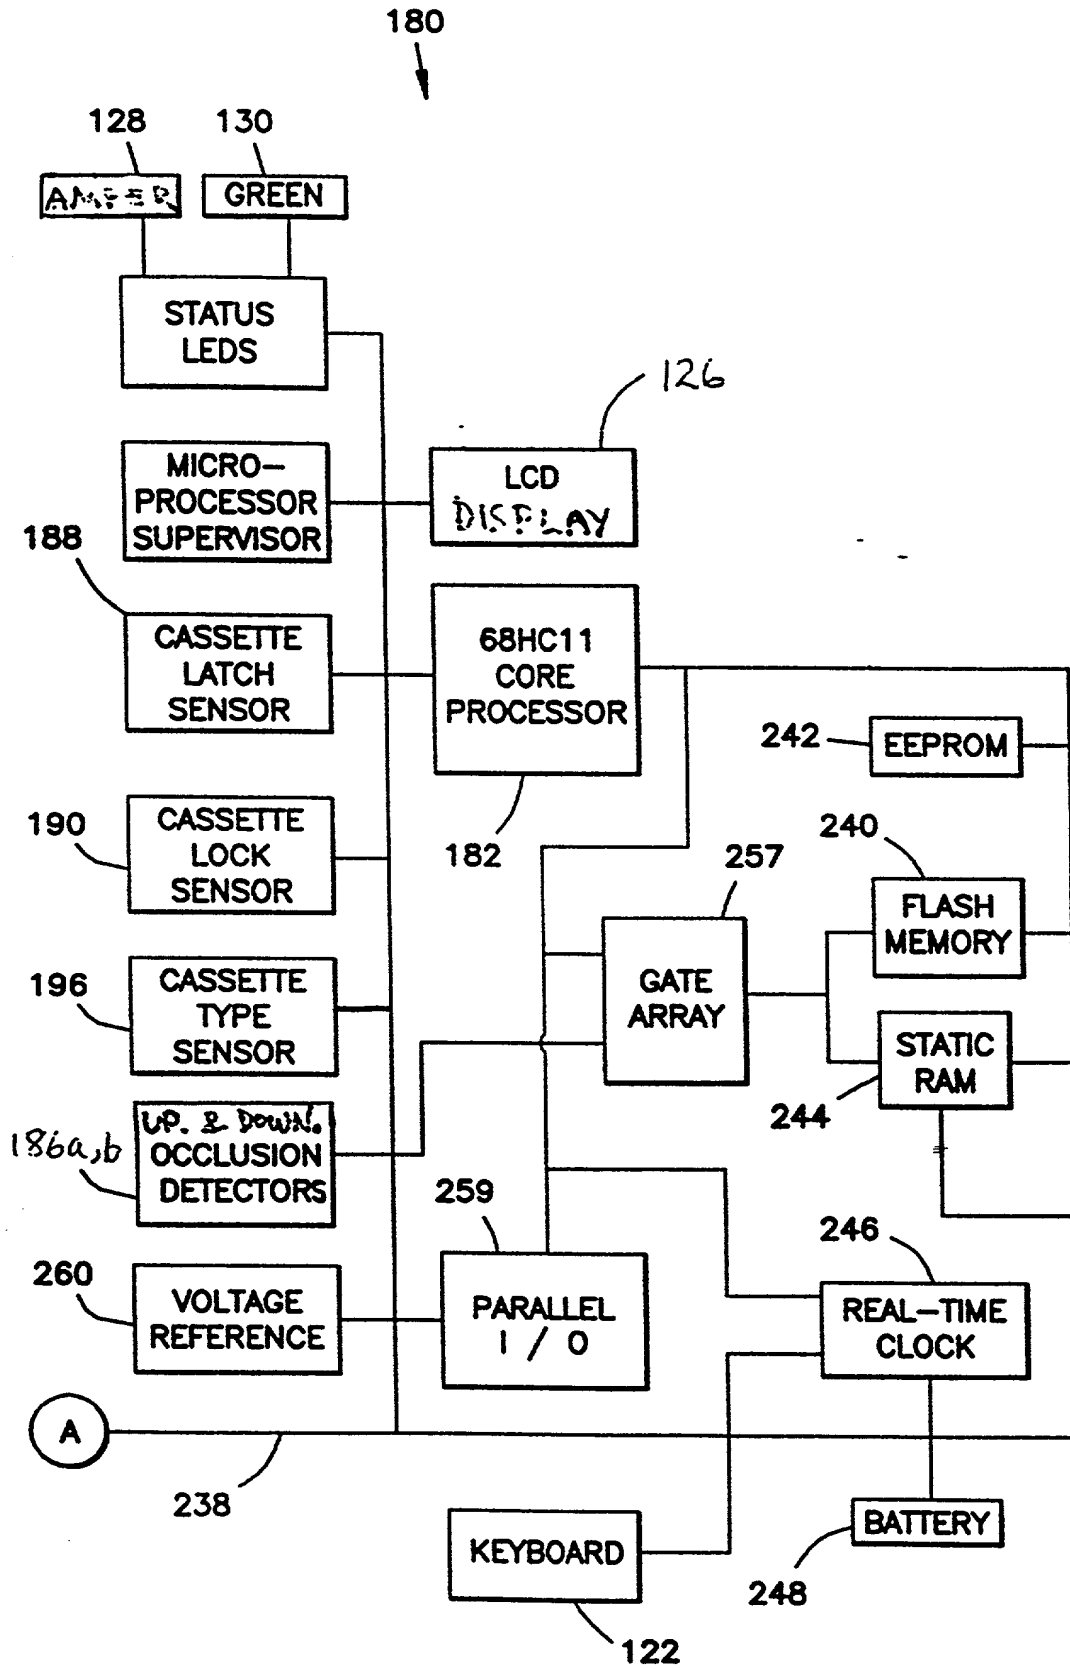


FIG. 8B

PCA APPLICATION INTERMITTENT TPN CONTINUOUS

PCA CODE	INTERMITTENT CODE	TPN CODE	CONTINUOUS CODE
PUMP APPLICATION TEMPLATE	PUMP APPLICATION TEMPLATE	PUMP APPLICATION TEMPLATE	PUMP APPLICATION TEMPLATE
PUMP KERNEL	PUMP KERNEL	PUMP KERNEL	PUMP KERNEL
SERIAL COM. PROTOCOL	SERIAL COM. PROTOCOL	SERIAL COM. PROTOCOL	SERIAL COM. PROTOCOL
PUMP DRIVERS	PUMP DRIVERS	PUMP DRIVERS	PUMP DRIVERS

BOOT SYSTEM TEST UTILITY

BOOT	TEST
PUMP KERNEL	PUMP KERNEL
SERIAL COM. PROTOCOL	SERIAL COM. PROTOCOL
PUMP DRIVERS	PUMP DRIVERS

CORE BANK 2417

F16 8C



22-141 50 SHEETS  
22-142 100 SHEETS  
22-144 200 SHEETS

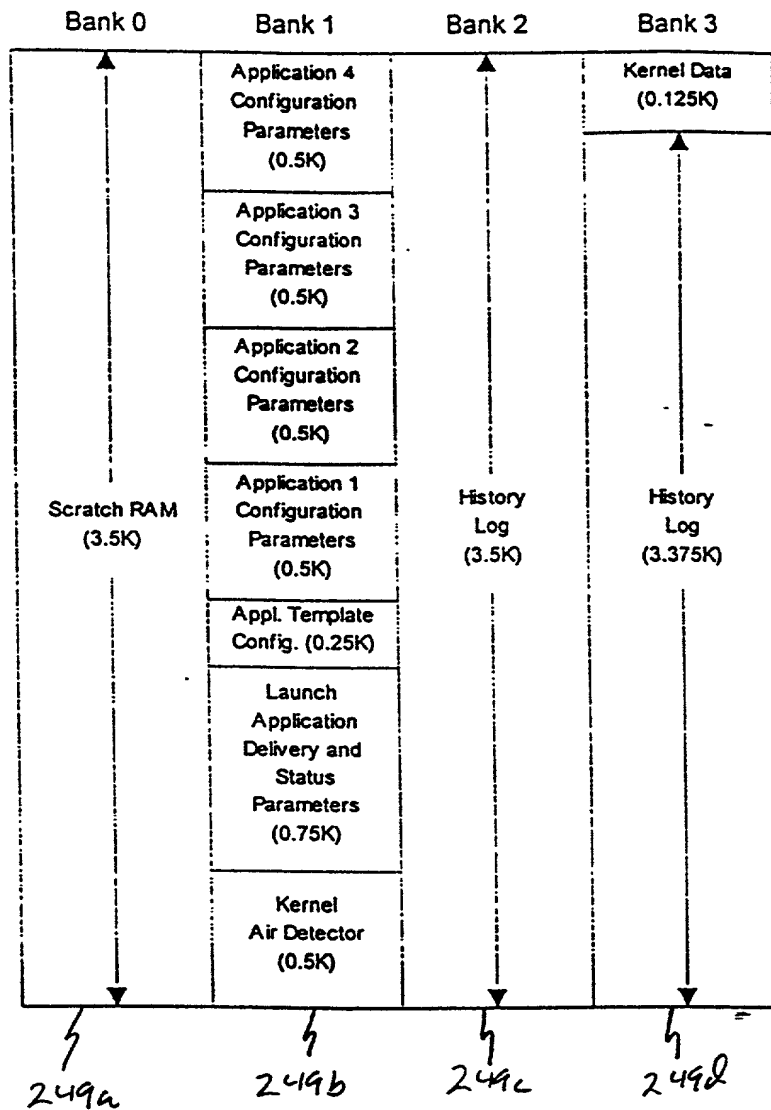


FIG 8D



242

App 4 Configuration Parameters
App 3 Configuration Parameters
App 2 Configuration Parameters
App 1 Configuration Parameters
App Template Configuration Parameters
Launch App Delivery/Status Parameters
KERNEL DATA: Automatic Odometers, Program Look-up Table, Launch Program Select, Kernel and App Need Defaulting flags.
DRIVERS DATA: Error Log
DRIVERS DATA: Manufacturing Parameters

FIG. 8E

203

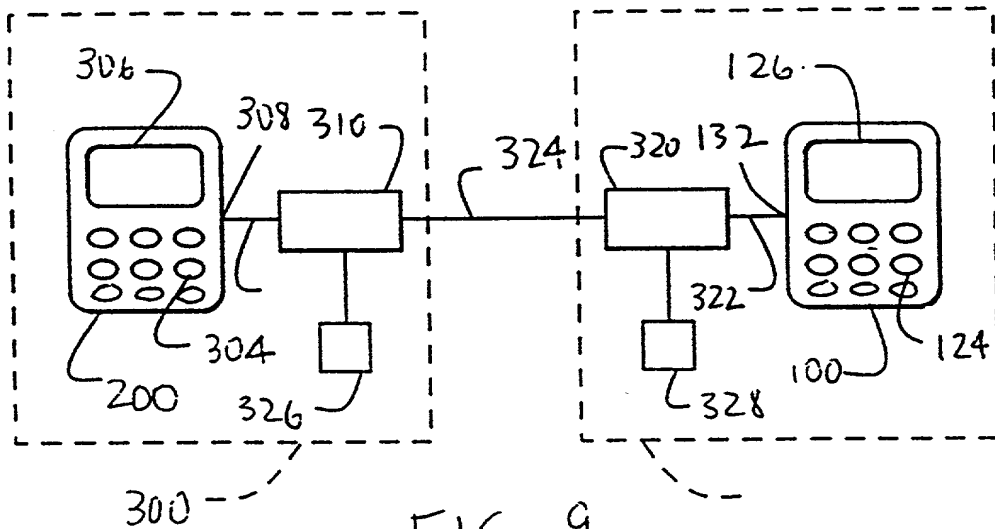


FIG. 9

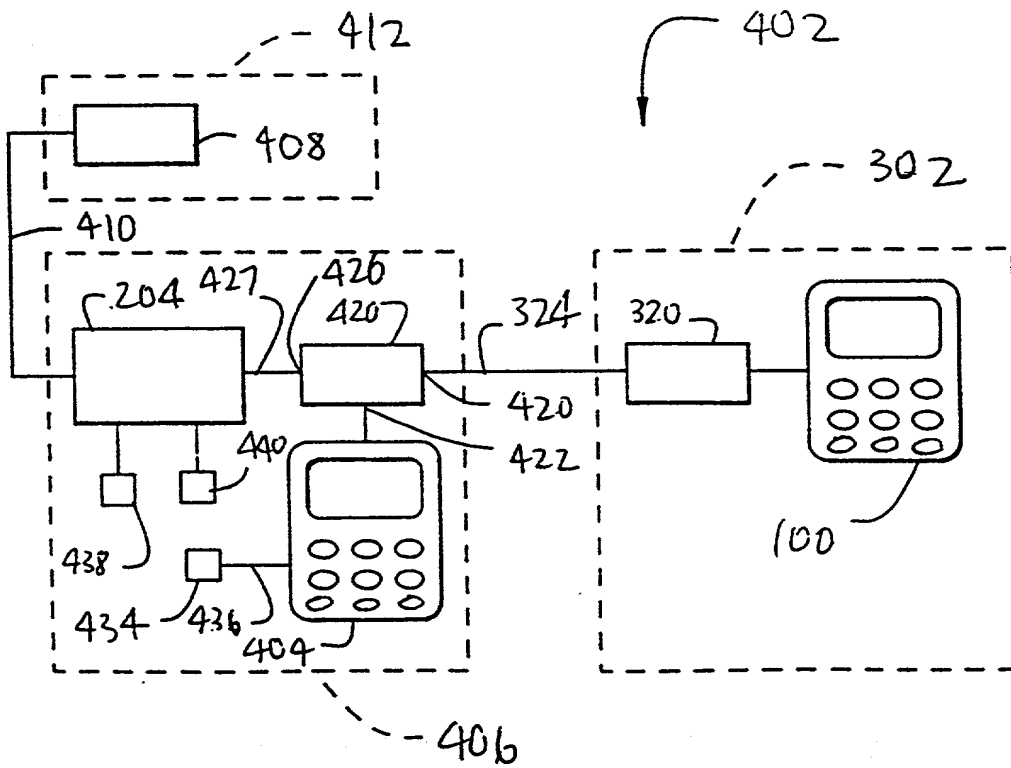


FIG. 10

421

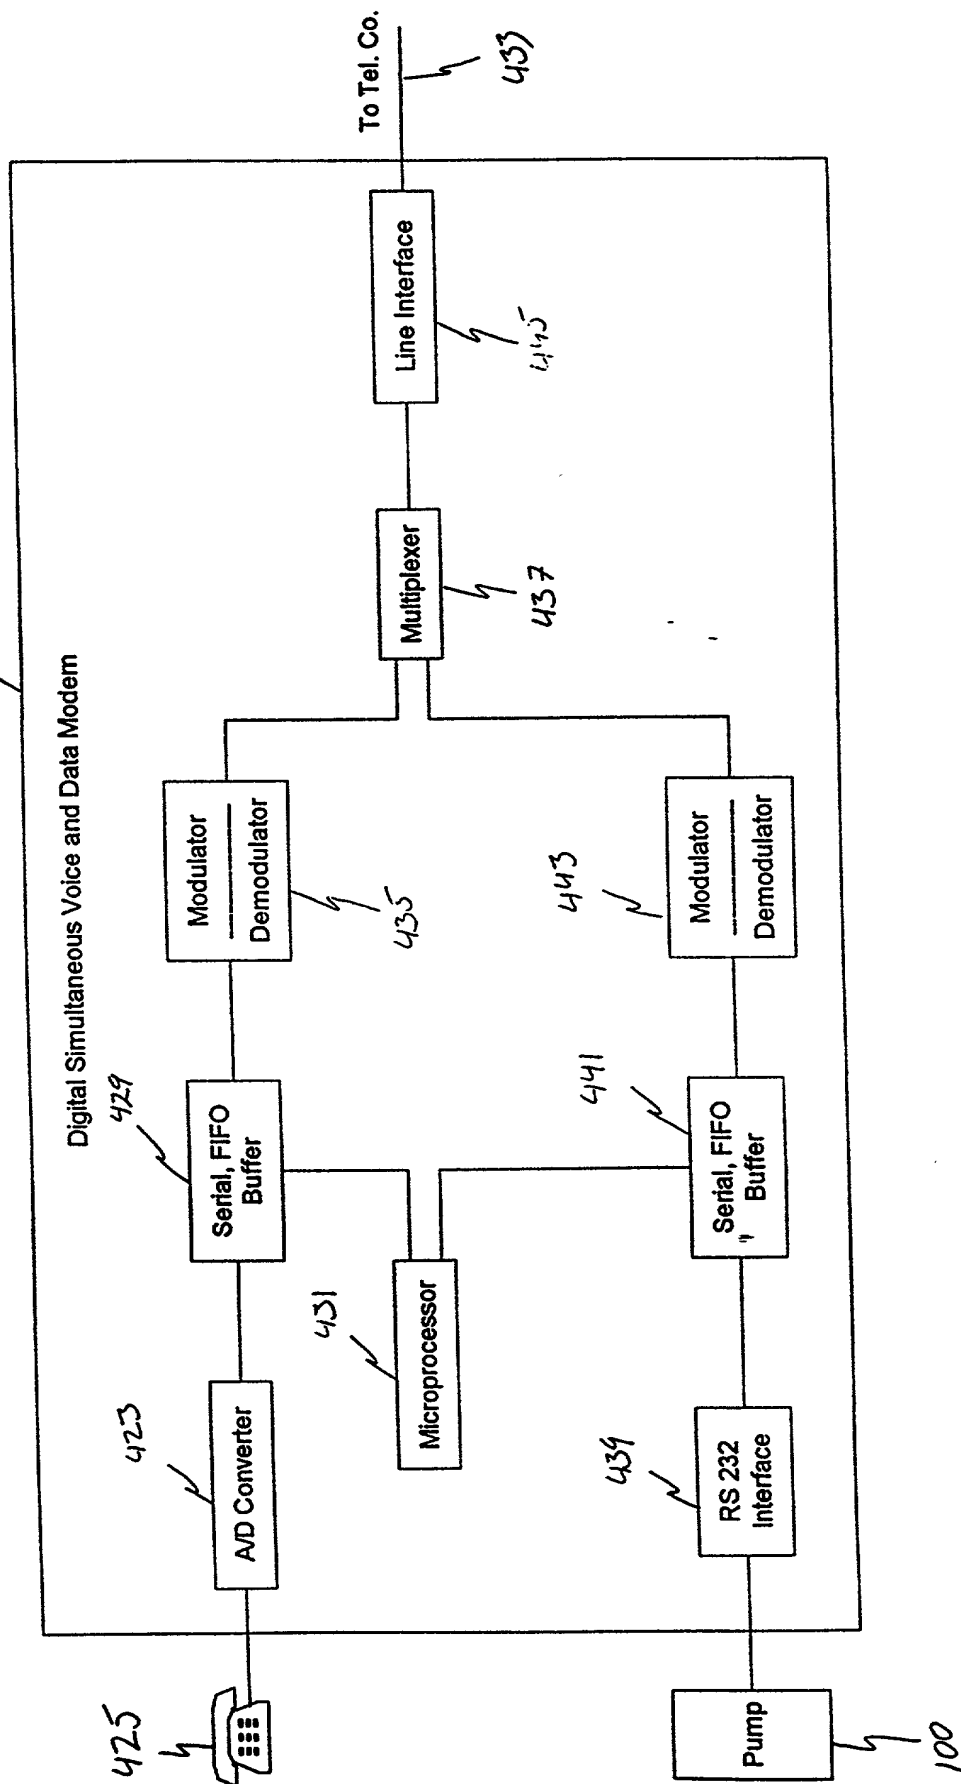


FIG. 11

380

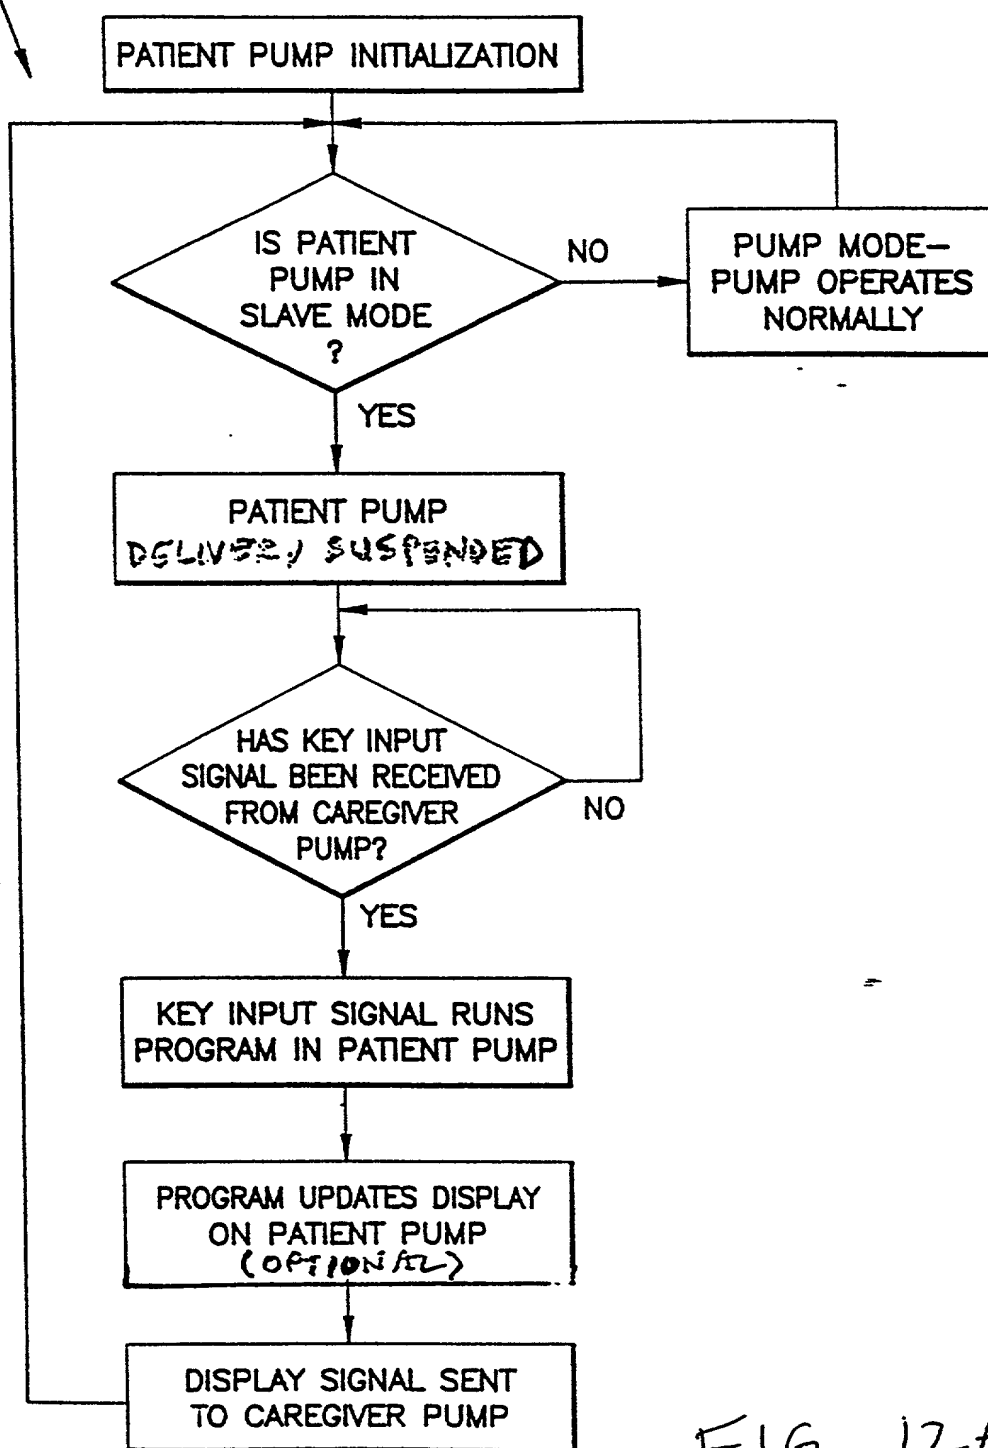


FIG. 12A

382

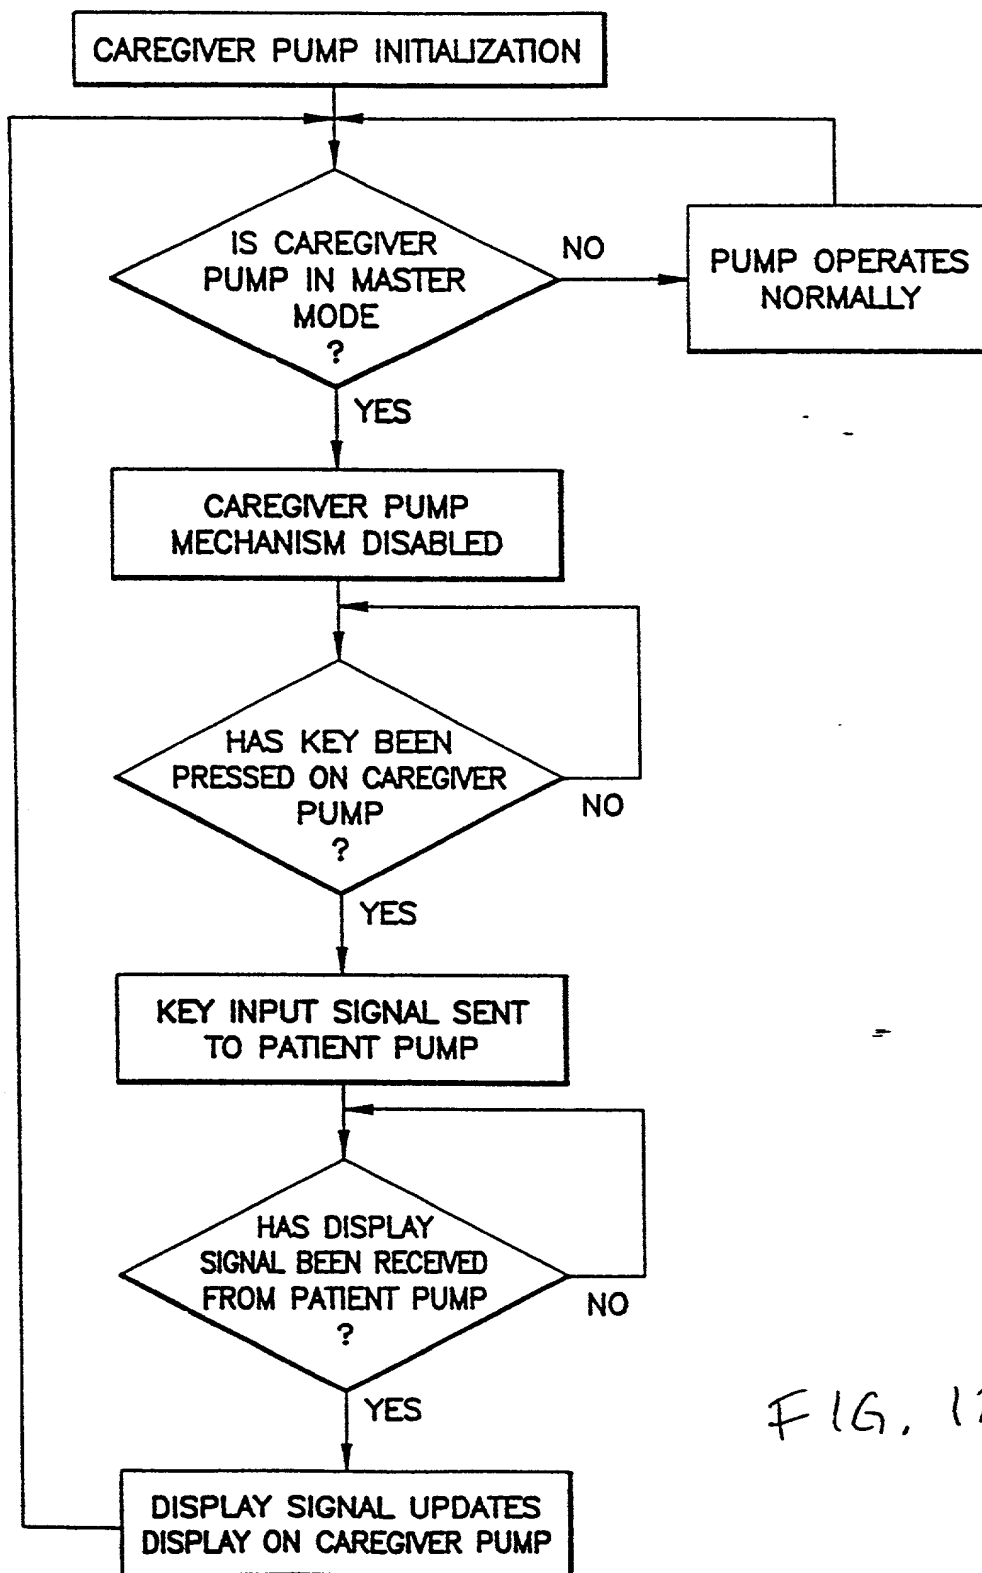


FIG. 12B

10069294 10069294

386                      384                      388

↓

CAREGIVER PUMP	PATIENT PUMP
Clinician's pump must be running the Terminal Application. If the communications cable is not connected, clinician attaches cable.	
Clinician talks with patient using phone connected to modem	Patient talks with clinician using phone connected to modem
Clinician instructs patient to "connect communications cable to patient's pump"	Patient connects cable to pump
After cable connected, clinician asks patient to "verify that the screen with CONNECT TO PHONE message is displayed"	Patient verifies screen
Clinician instructs patient to "select CONNECT TO PHONE option, wait for a tone, then hang up phone and wait for a call back (call back is optional)".	Patient selects option, listens for tone, then hangs up phone. Patient's pump reminds patient to hang up phone.
Clinician listens for tone from patient's pump, then presses a key on Clinician's pump.	Patient waits for clinician to call back.
Clinician's pump and patient's pump connect	Patient's pump displays a standard message and all key beeps are suppressed
Clinician reviews/modifies patient's pump.	
Clinician logs-off	Patient's pump begins to periodically alarm. Message instructs patient to remove modem cable
Clinician calls patient (Optional)	

FIG. 13

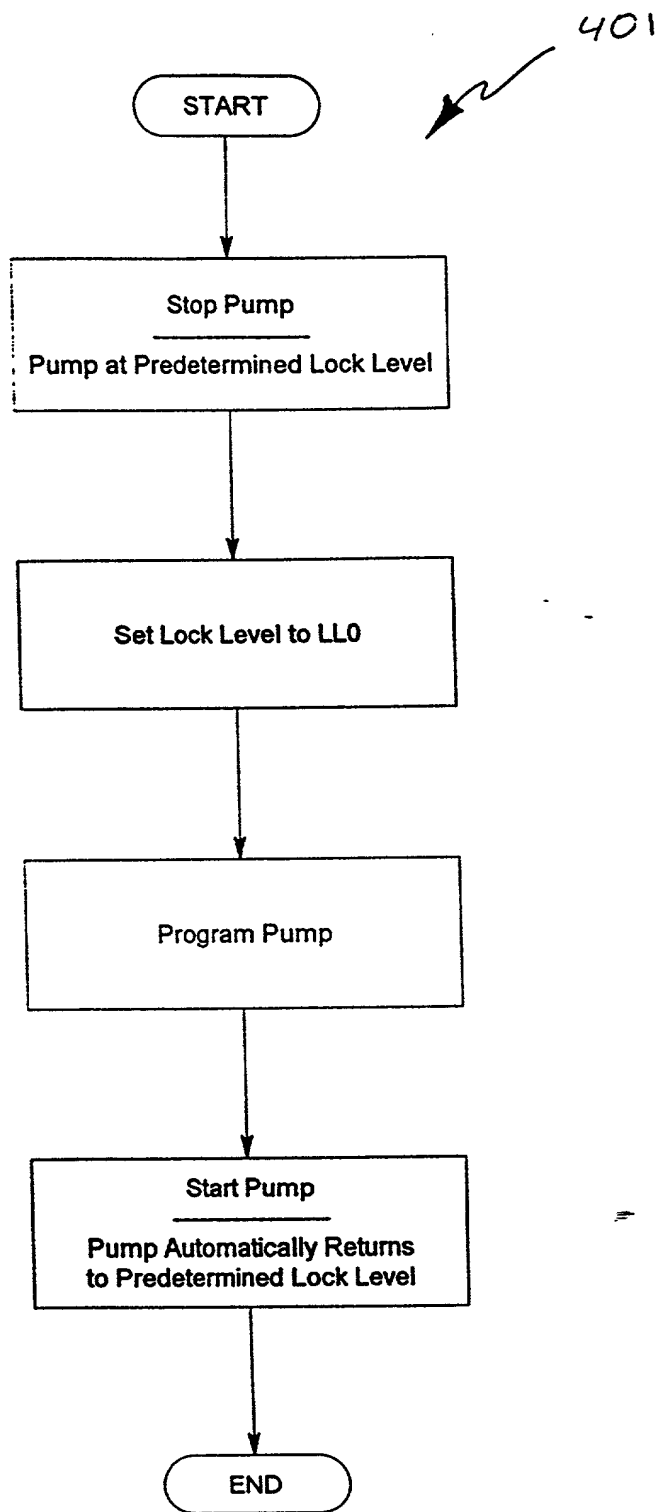
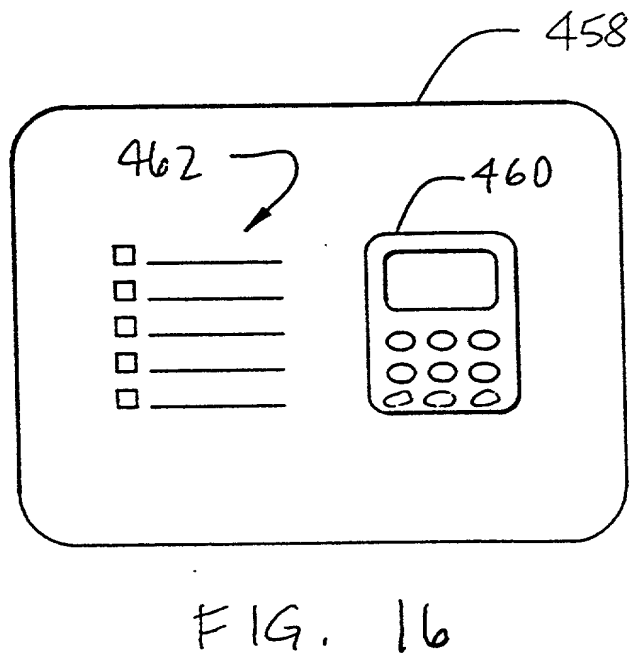
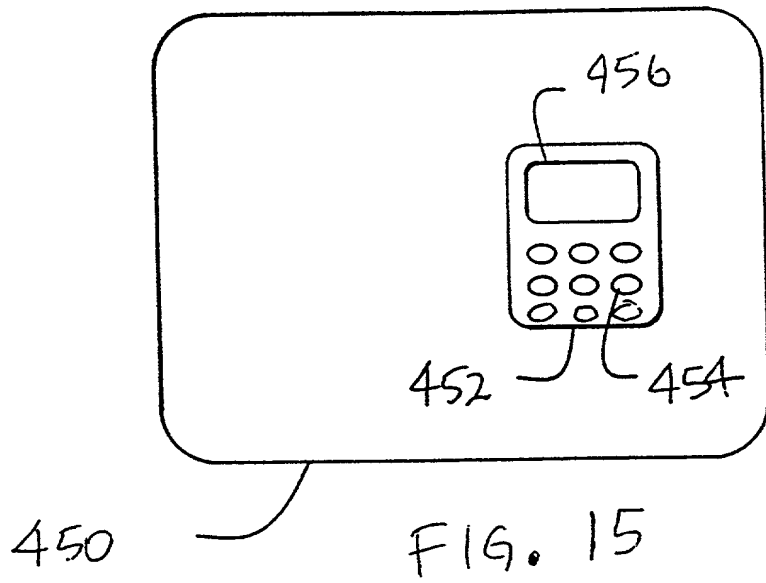


FIG. 14

10065294 020400





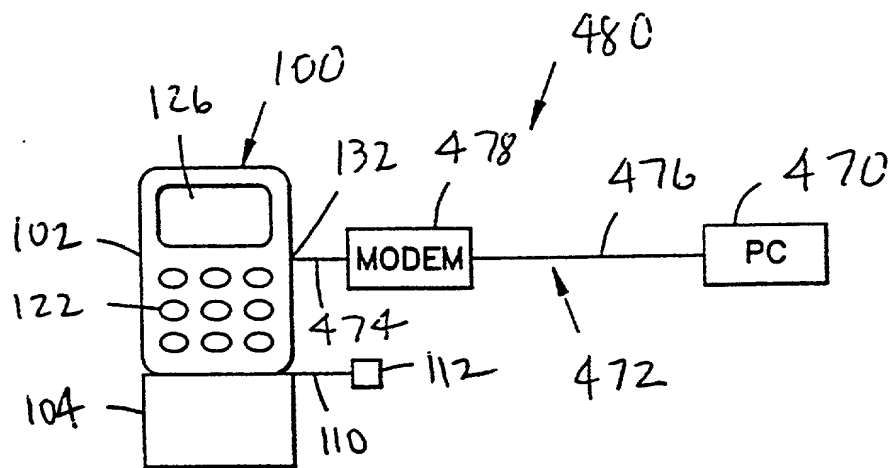


FIG. 17

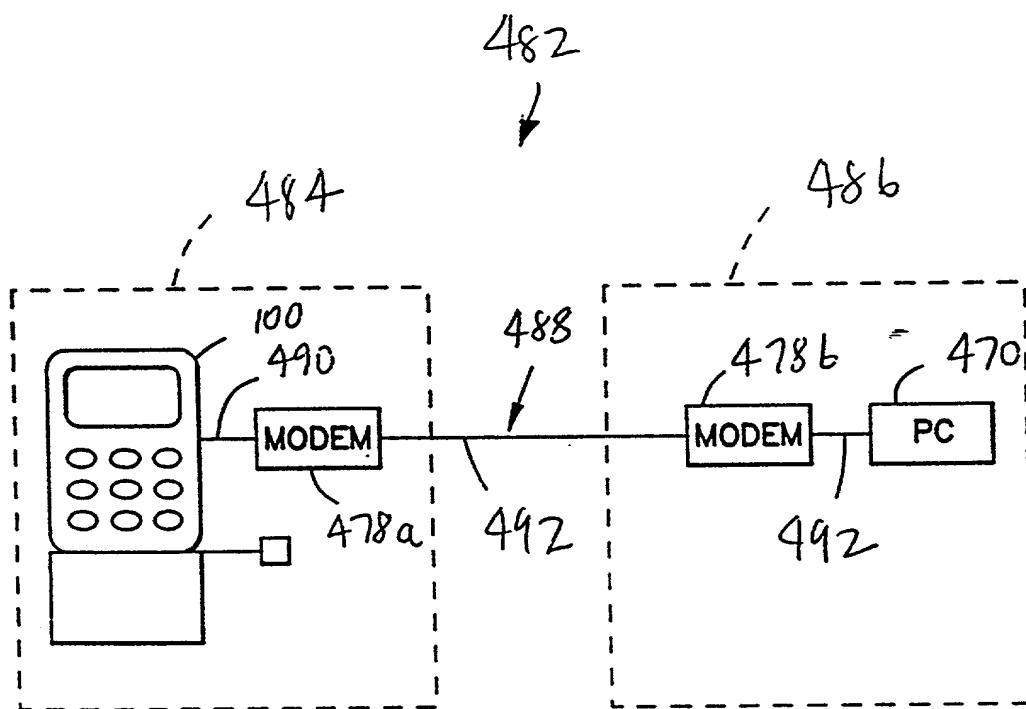


FIG. 18

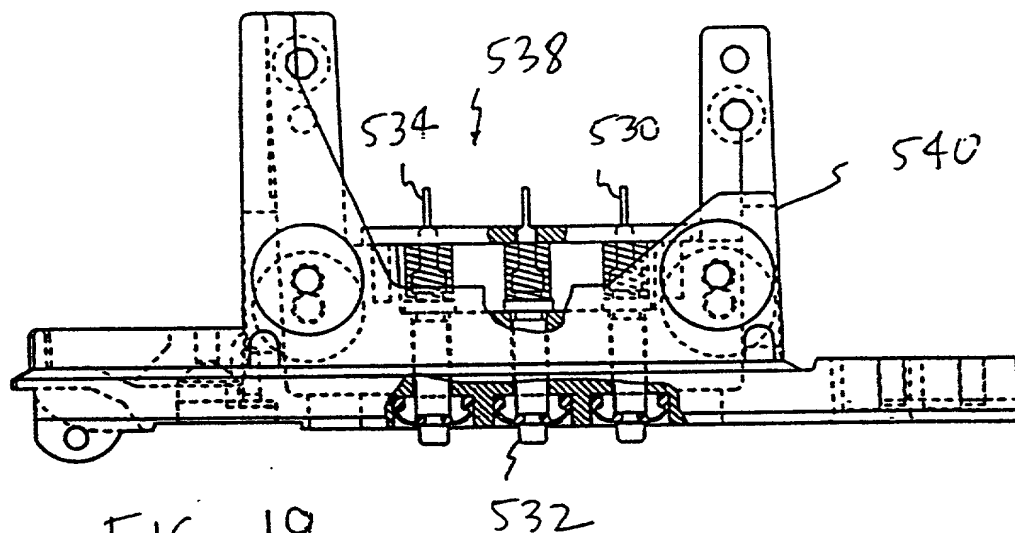


FIG. 19

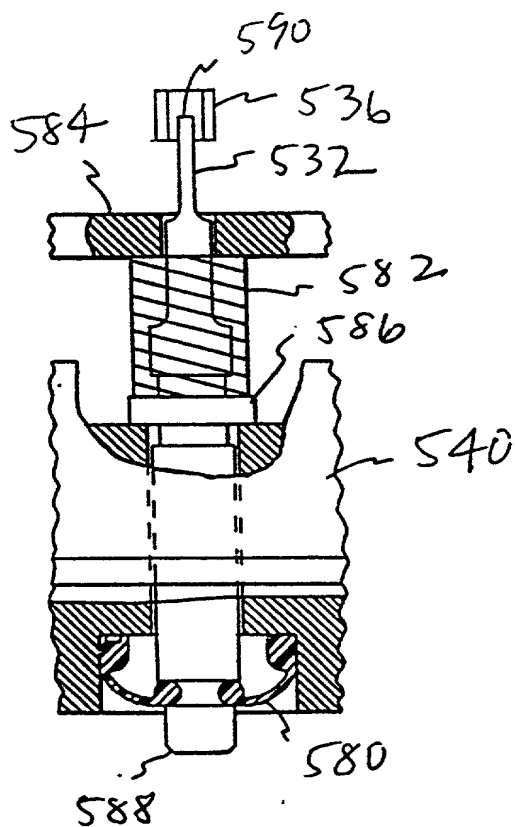


FIG. 20

40068294.000502

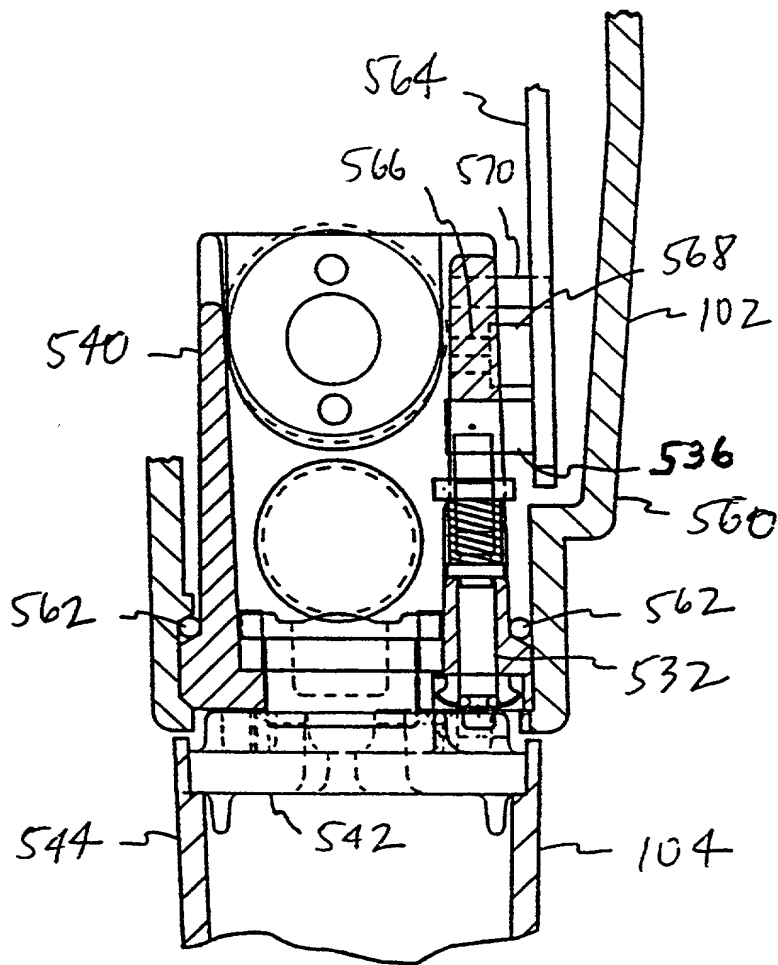
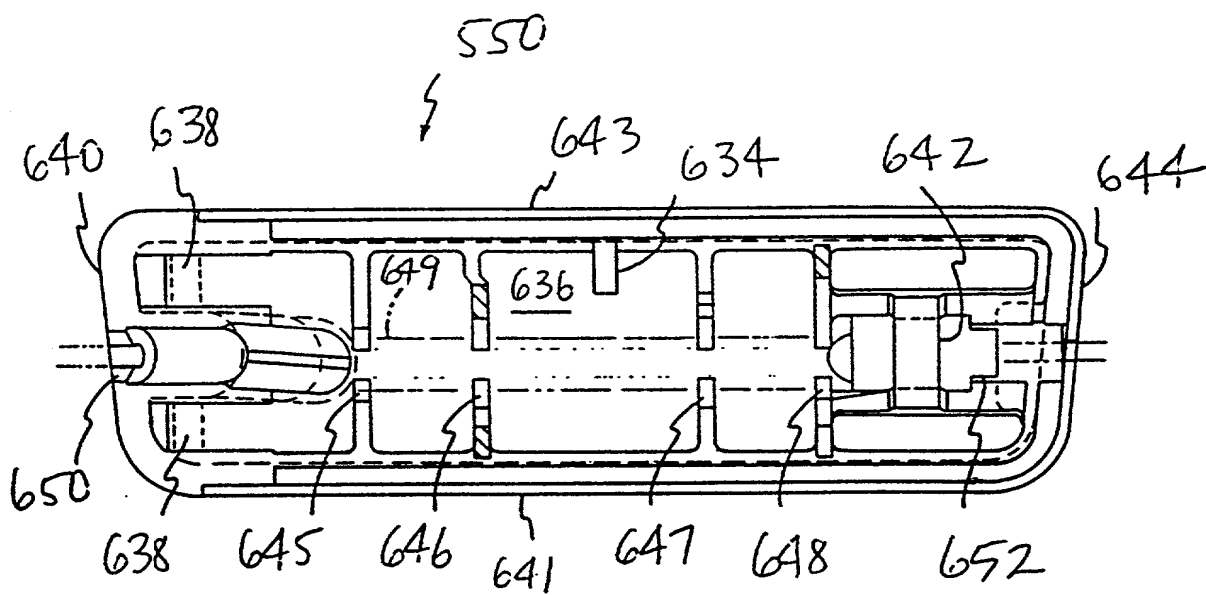
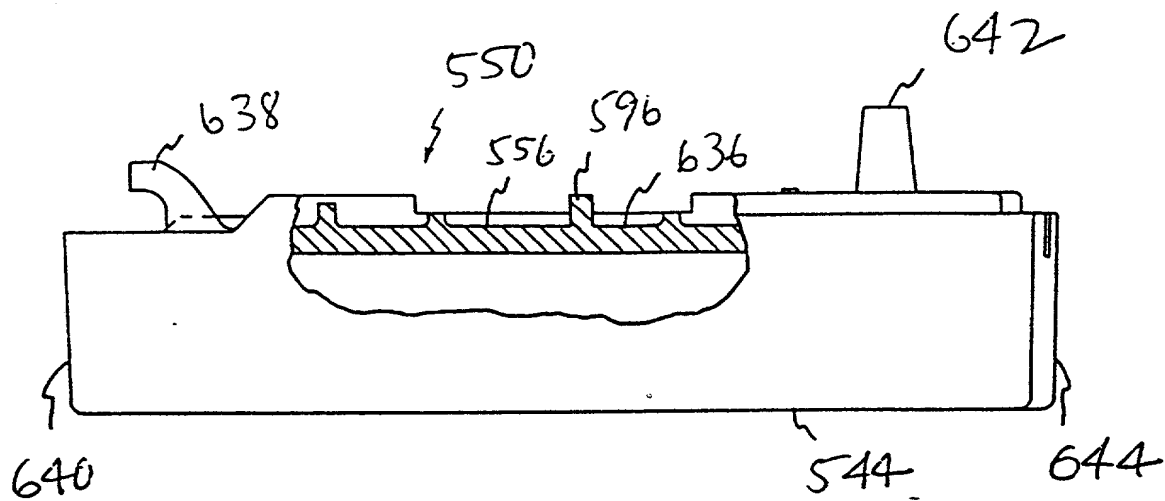
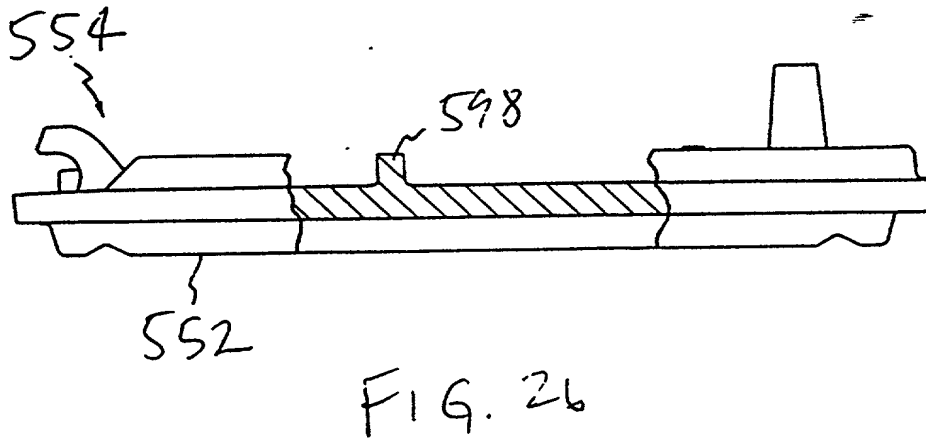
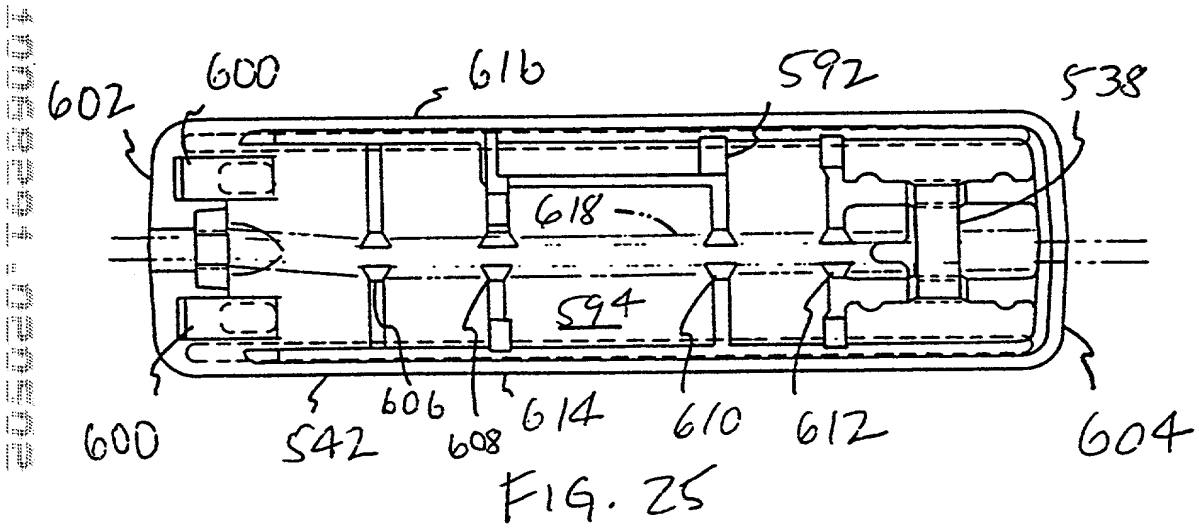
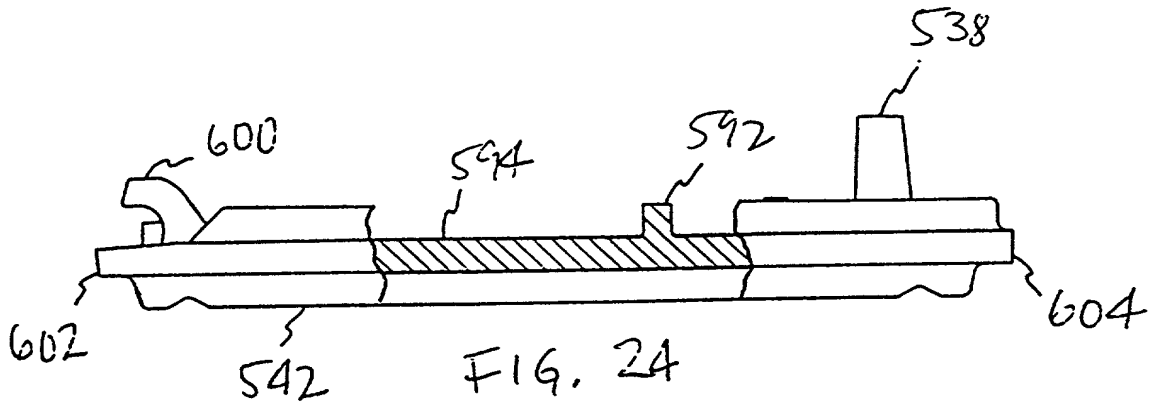


FIG. 21





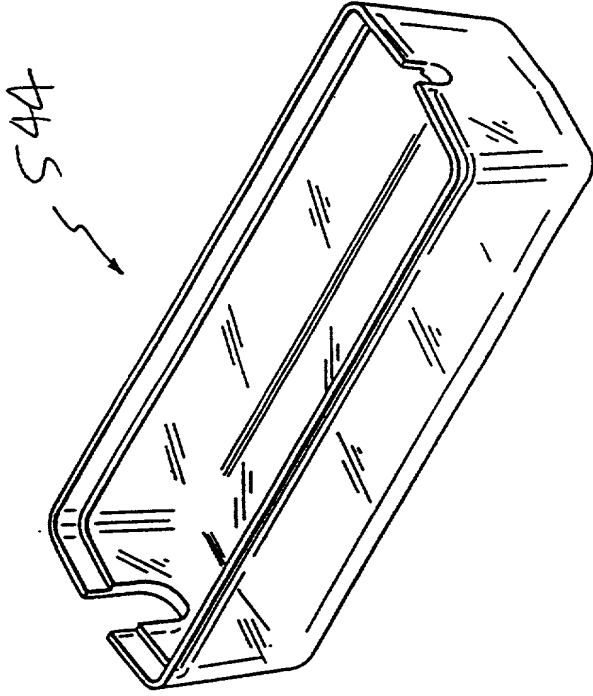


FIG. 27

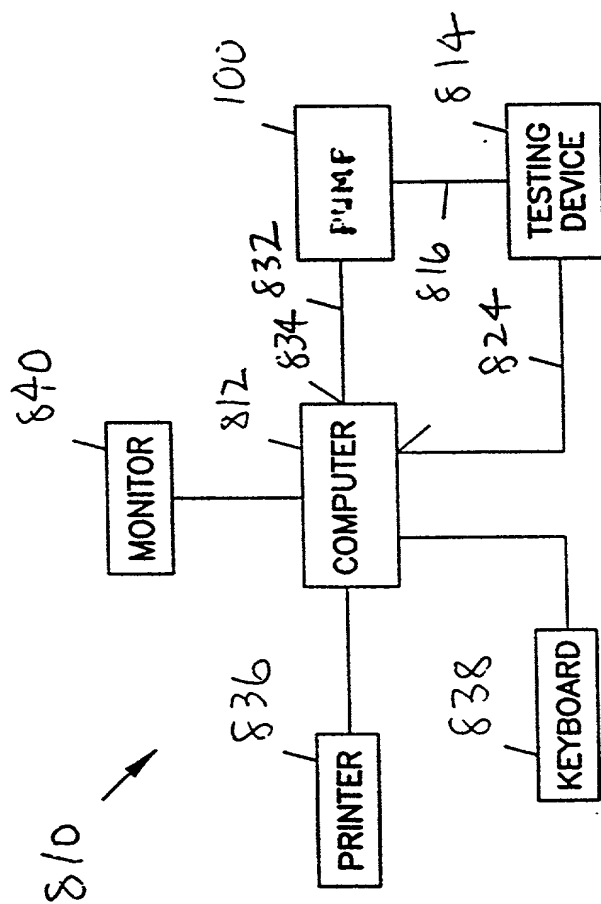


Fig. 28

208

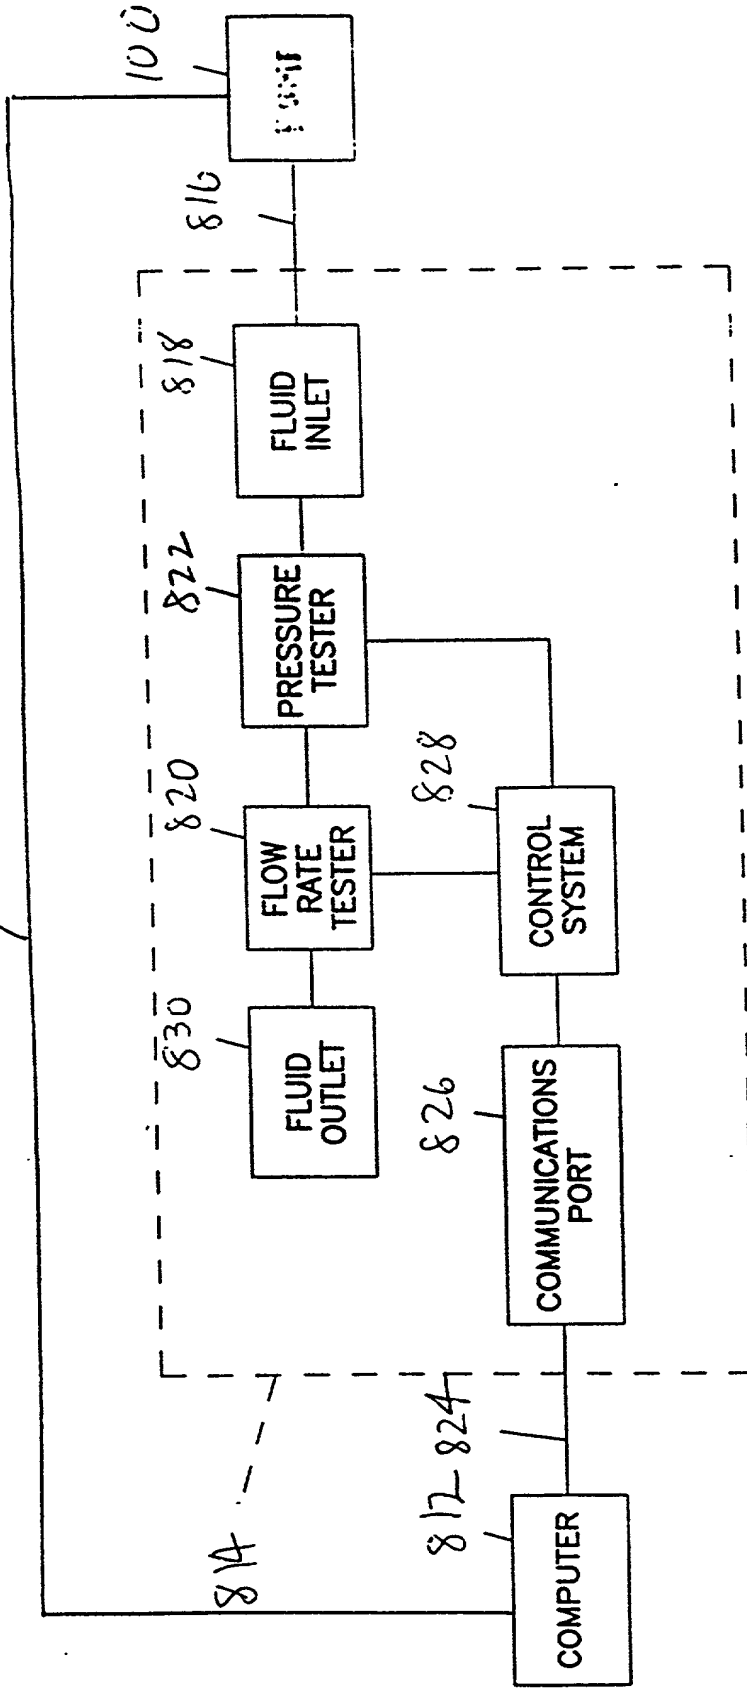


FIG. 29



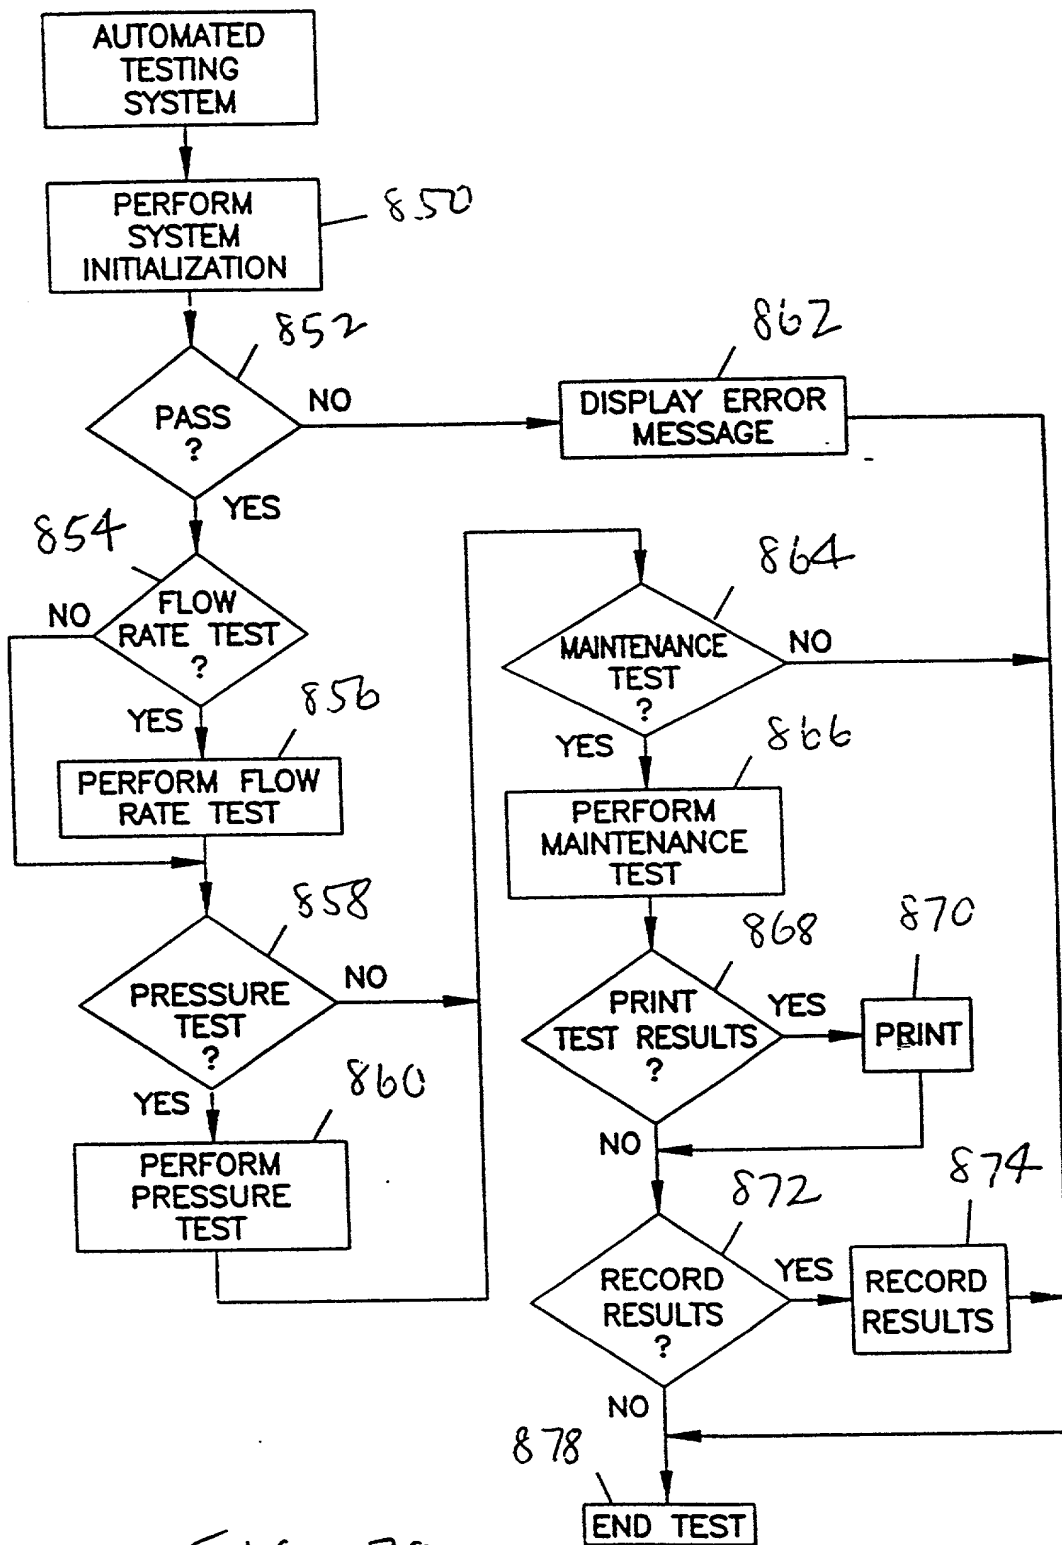


FIG. 30

40068294 00000000

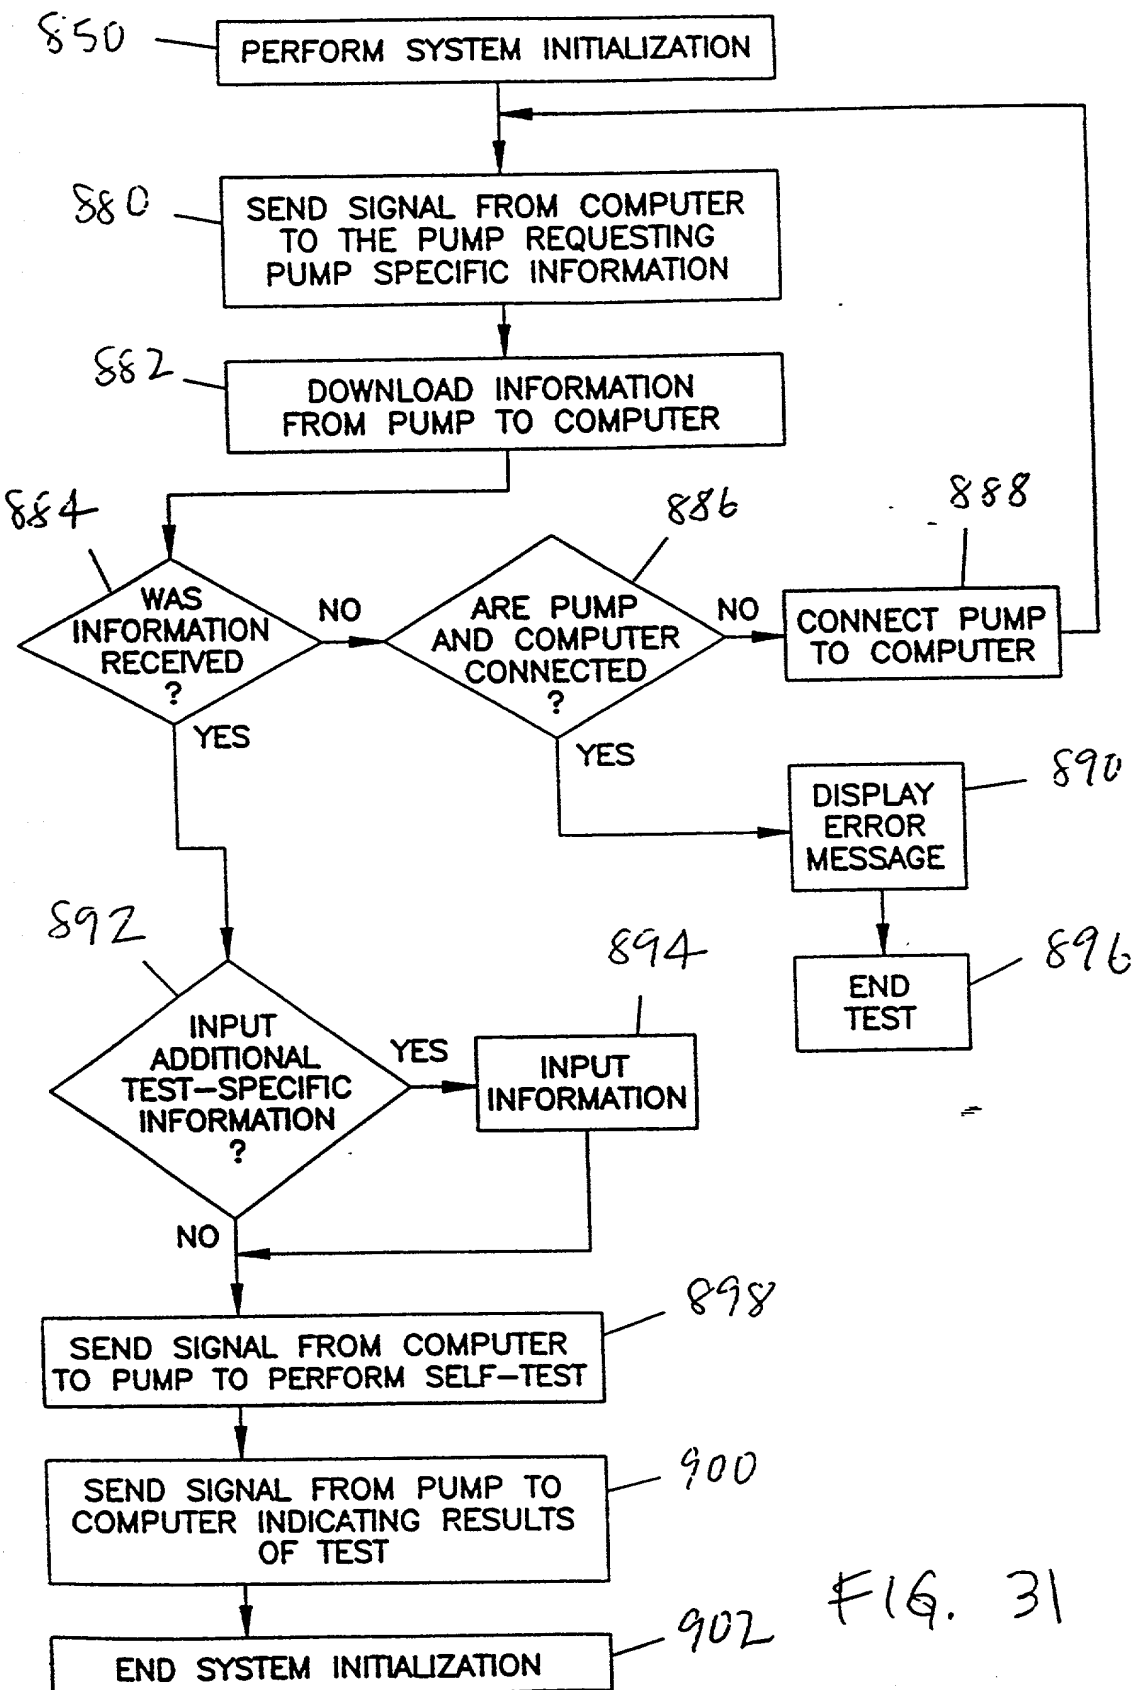


FIG. 31

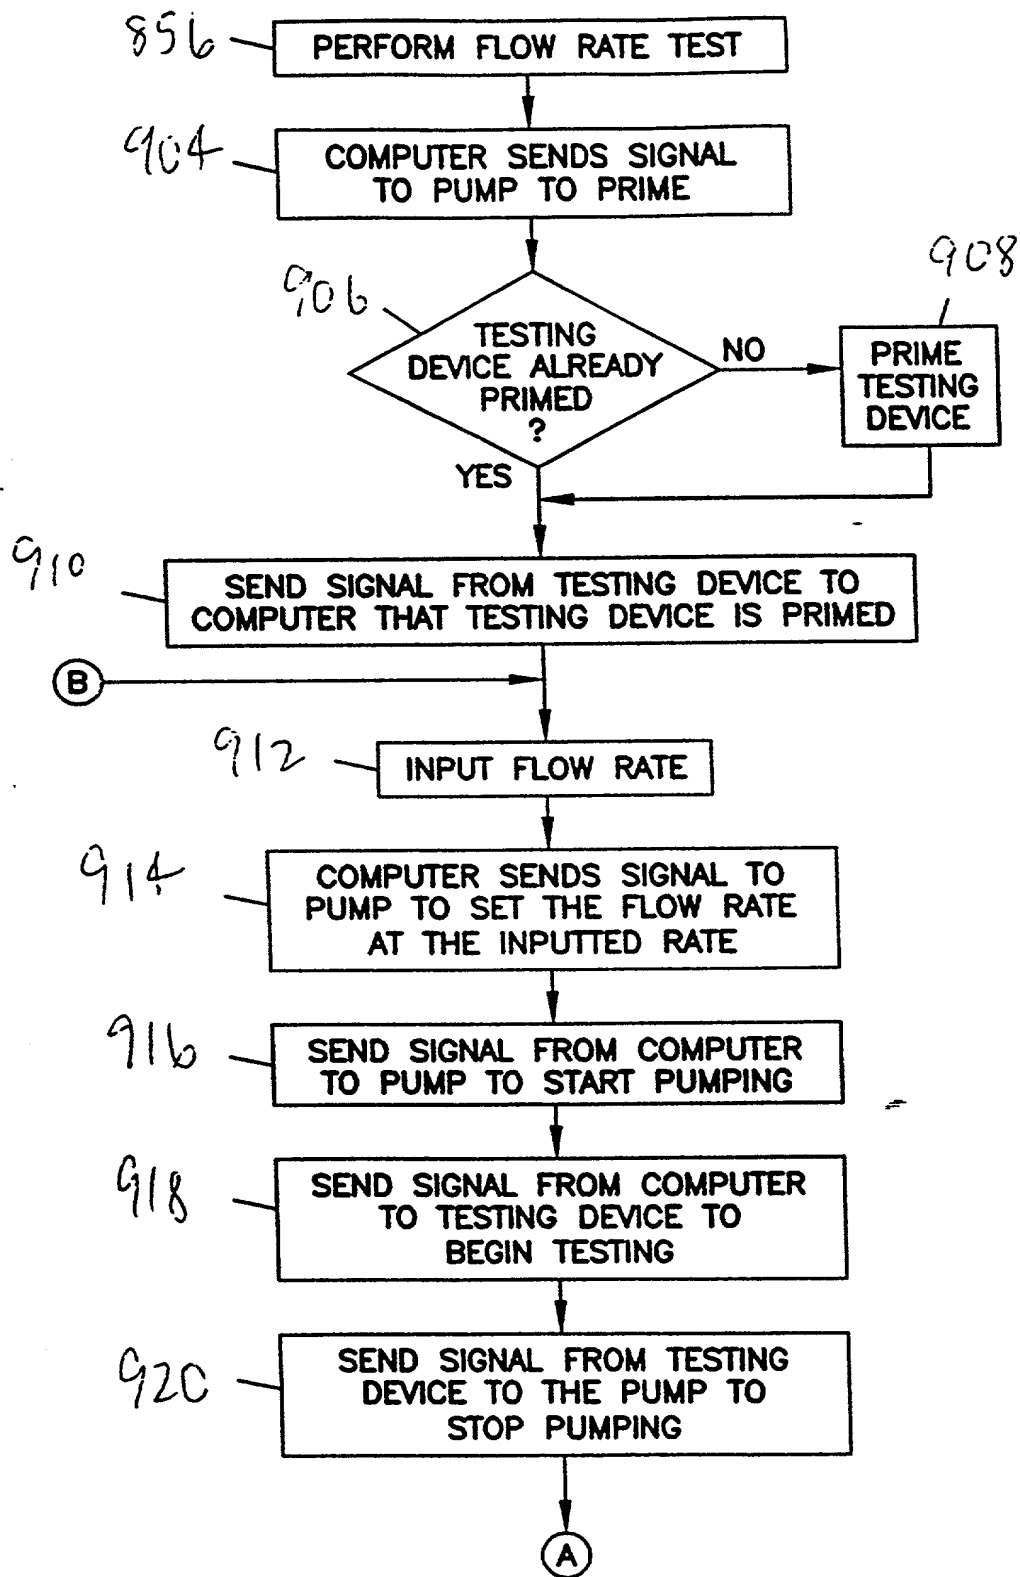


FIG. 32A

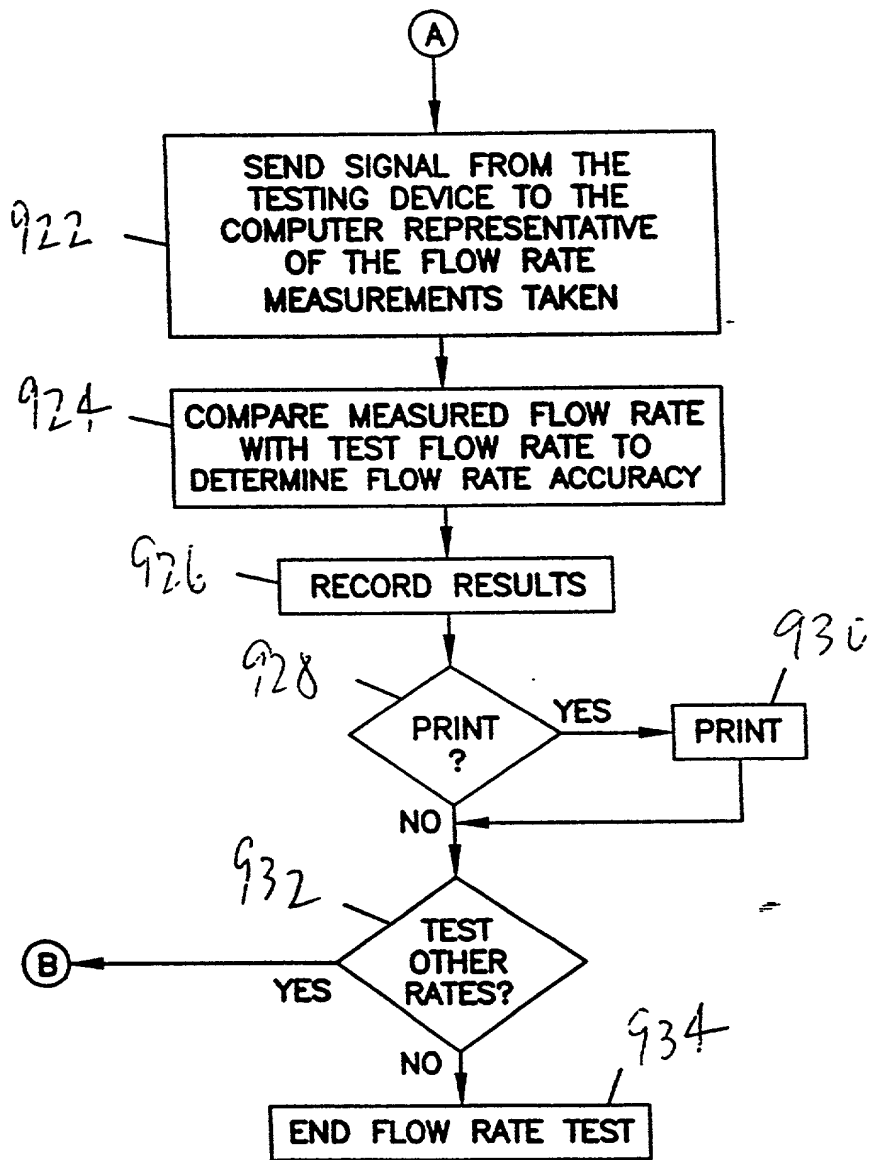


FIG. 32B

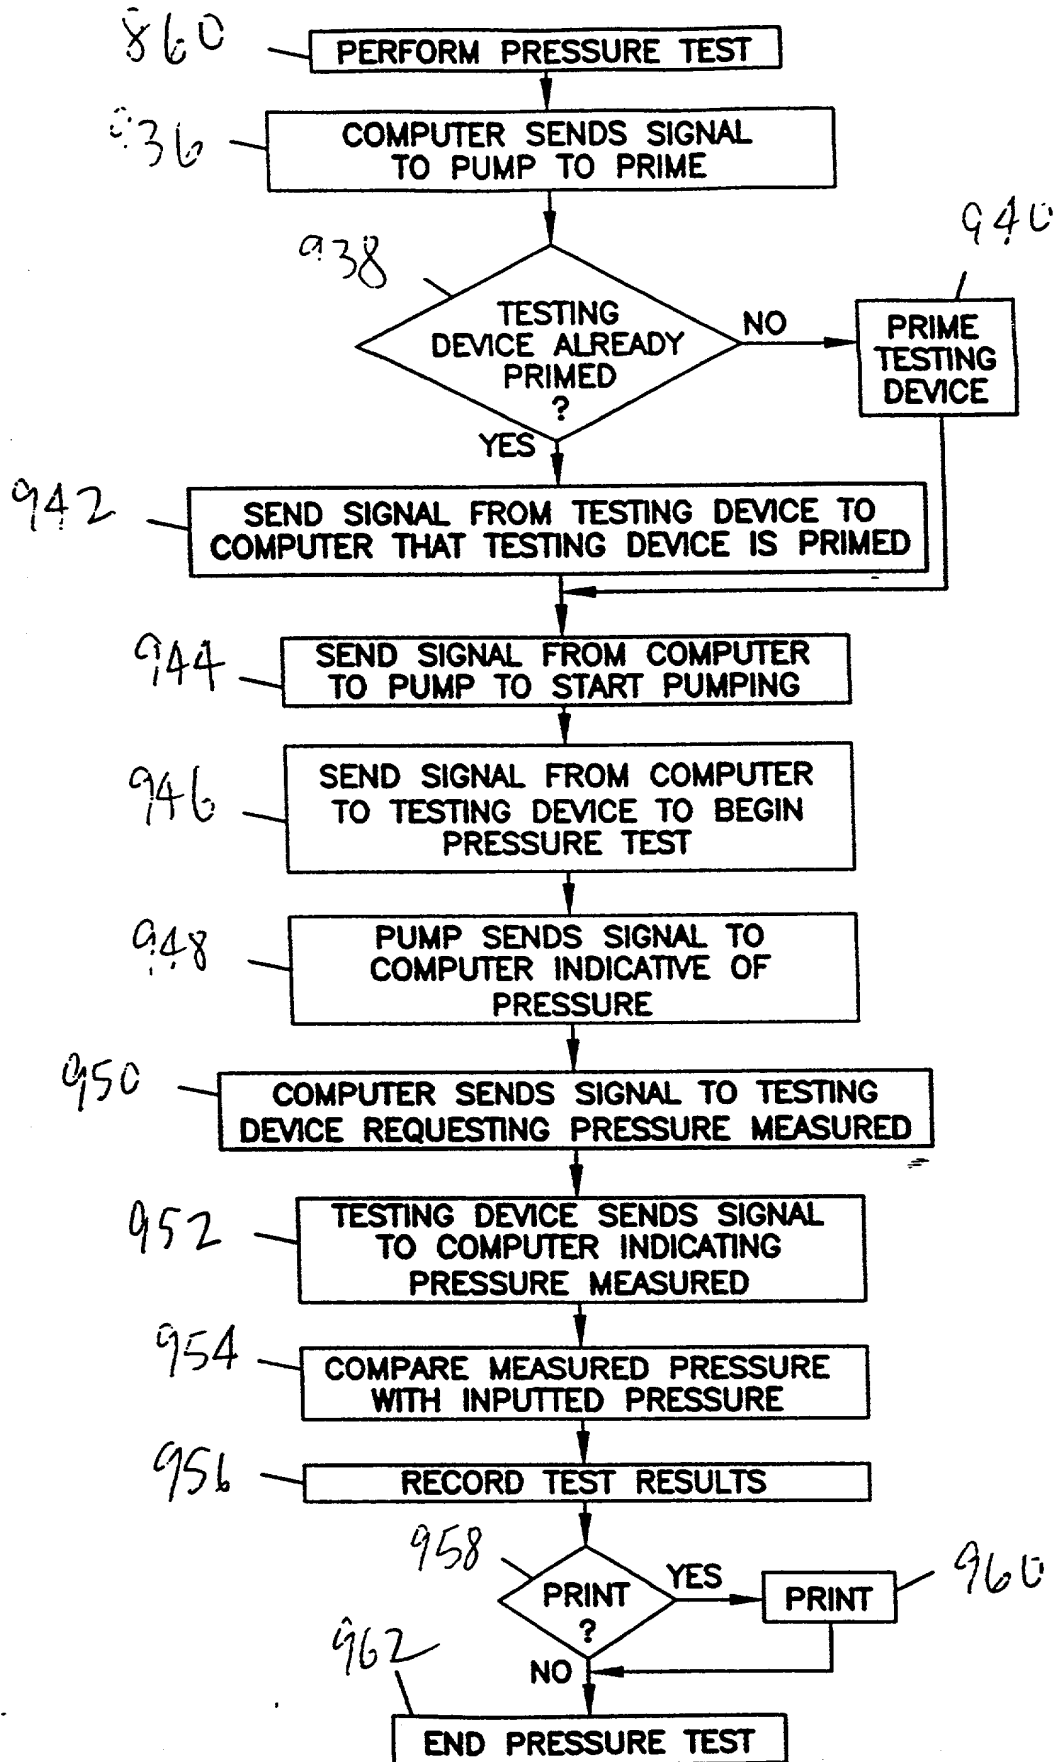


FIG. 33

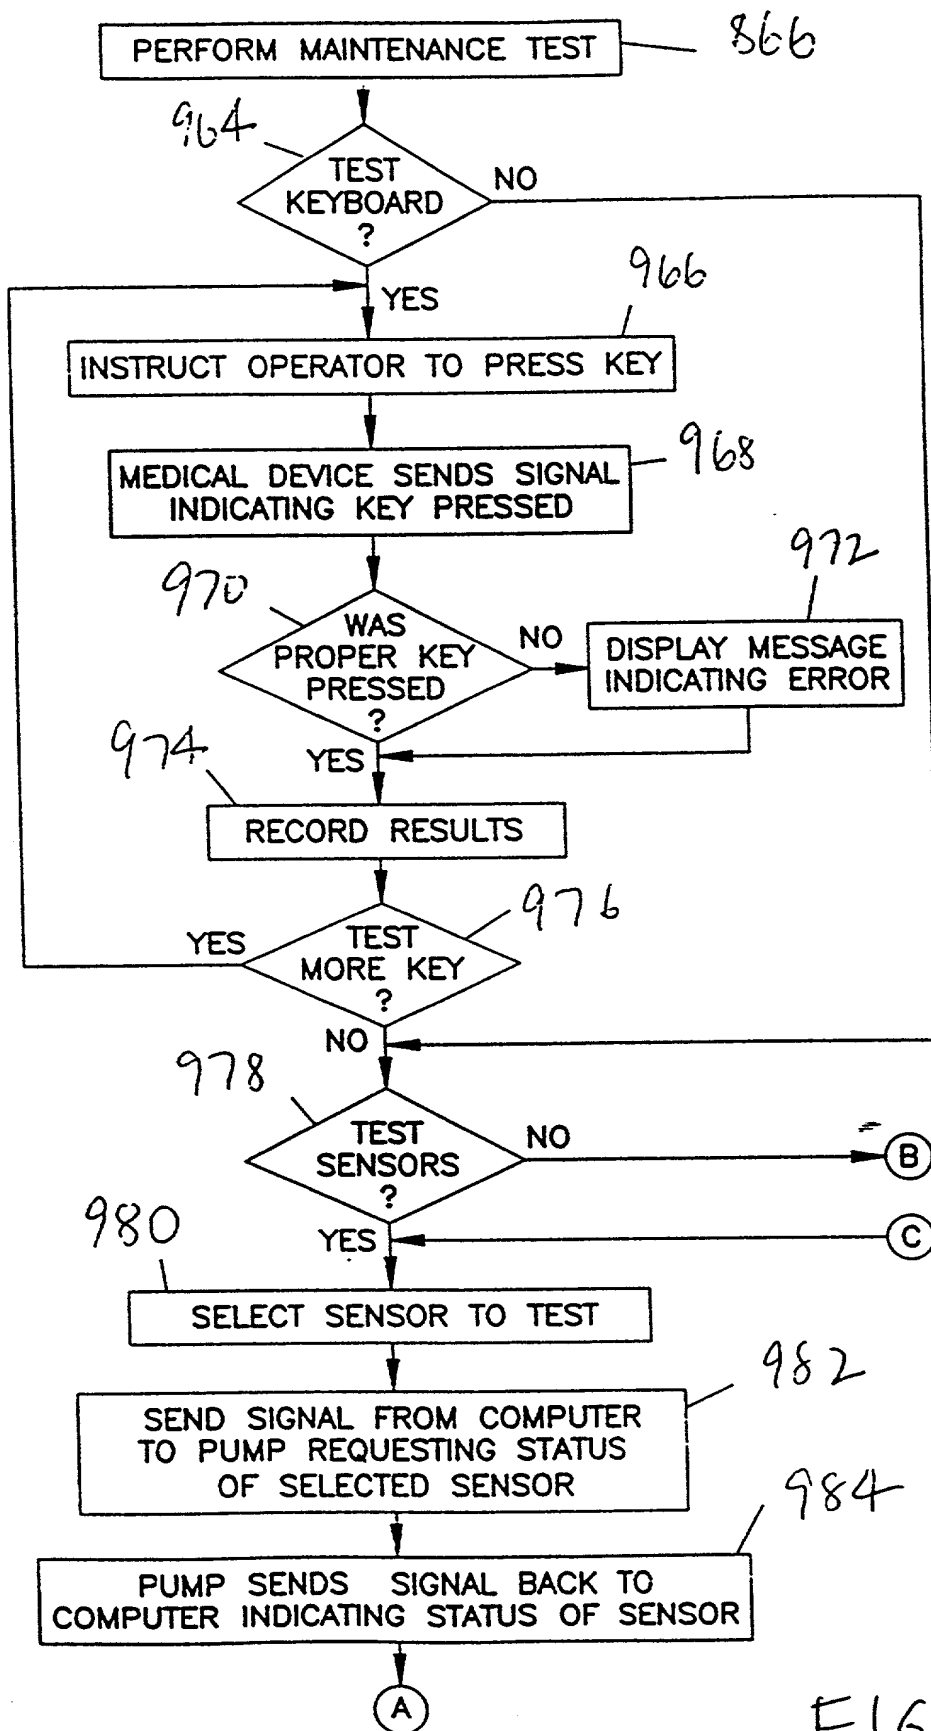


FIG. 3A

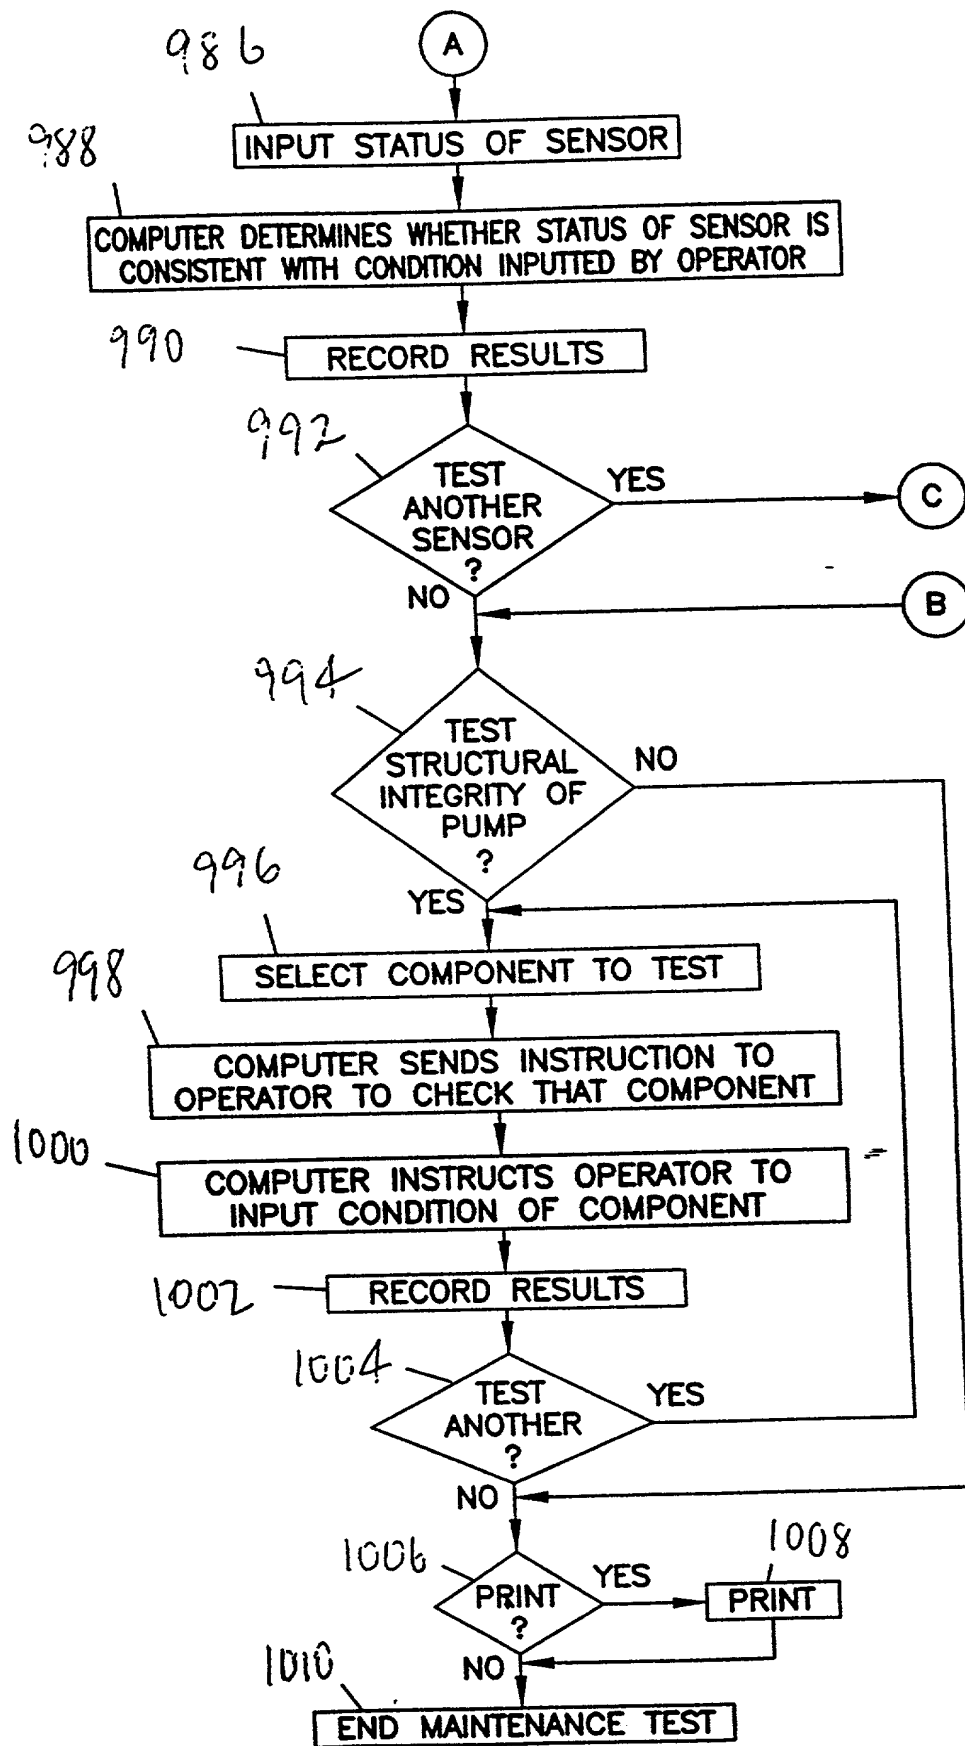


FIG. 34 B